



Roller Oven Calibration Report


Order Number:	0023144
Serial # / Local I.D. #:	00-11
Calibration Date:	3/9/2026
Recommended Due Date:	3/9/2027
Certificate Number:	00-1146090
Manufacturer:	OFI Testing Equipment
Part Number:	174-00

Condition Found:	In Calibration
Condition Left:	In Calibration
Repairs Required:	No
Static Oven:	No
(F) or (C):	(°F)
Max Temp:	400
As Found Required:	No

OFI Testing Equipment, Inc. - 11302 Steeplecrest Dr - Houston, Texas - 77065 - Phone: 832.320.7300 - Web: www.ofite.com

Calibration Equipment						
Thermometer	154	EA10	Z375331	C-52617	7/23/2025	7/23/2026
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Tachometer	706	R7050	220502483	C-54329	9/5/2025	9/5/2026
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Ambient Monitor	728	RH300	Z430119	305923	4/1/2025	4/1/2026
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Ambient Conditions	Lab / Room Temperature		72.8	(°F)	Lab / Room Humidity 53.4 %	

AS LEFT MEASUREMENTS		(°F)	Max Oven Temp	400	
Set point	Process Temperature	Accepted Deviation	Actual Deviation	Pass/Fail	
100.0	99.0	5.0	-1.0	Pass	
	Pass				
200.0	202.0	5.0	2.0	Pass	
	Pass				
300.0	303.0	5.0	3.0	Pass	
	Pass				
400.0	396.0	5.0	-4.0	Pass	
	Pass				
25 RPM	25	2	0	Pass	
	Pass				

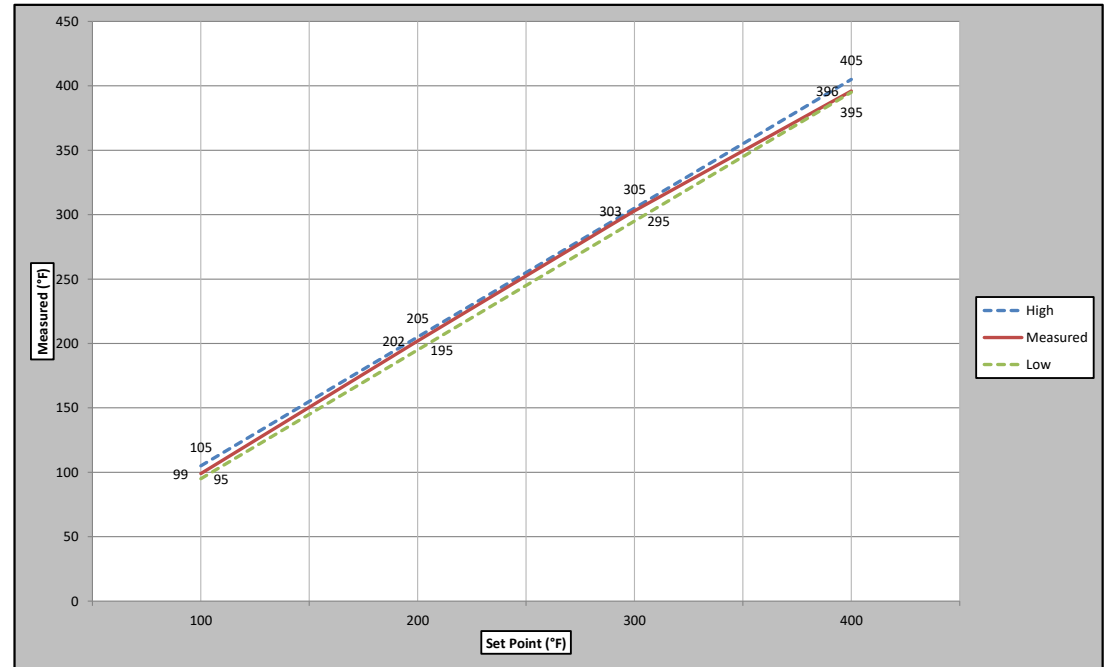

Calibration Technician: Shawn Maglitto

Technician Signature: *Shawn Maglitto*

Date: 3/9/2026

Reviewed By: Samantha Korenek

Reviewer Signature: *Samantha Korenek*

Review Date: 3/10/2026