



Roller Oven Calibration Report


Order Number:	0023041
Serial # / Local I.D. #:	12-06
Calibration Date:	12/9/2025
Recommended Due Date:	12/9/2026
Certificate Number:	12-0646000
Manufacturer:	OFI Testing Equipment
Part Number:	172-00-RC

Condition Found:	In Calibration
Condition Left:	In Calibration
Repairs Required:	No
Static Oven:	No
(F) or (C):	(°F)
Max Temp:	400
As Found Required:	No

OFI Testing Equipment, Inc. - 11302 Steeplecrest Dr - Houston, Texas - 77065 - Phone: 832.320.7300 - Web: www.ofite.com

Calibration Equipment						
Thermometer	154	EA10	Z375331	C-52617	7/23/2025	7/23/2026
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Tachometer	173	461920	131105905	C-46744	2/6/2025	2/6/2026
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Ambient Monitor	728	RH300	Z430119	305923	4/1/2025	4/1/2026
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Ambient Conditions	Lab / Room Temperature		72.6	(°F)	Lab / Room Humidity 38.7 %	

AS LEFT MEASUREMENTS		(°F)	Max Oven Temp	400	
Set point	Process Temperature	Accepted Deviation	Actual Deviation	Pass/Fail	
100.0	102.0	5.0	2.0	Pass	
	Pass				
200.0	203.0	5.0	3.0	Pass	
	Pass				
300.0	304.0	5.0	4.0	Pass	
	Pass				
400.0	404.0	5.0	4.0	Pass	
	Pass				
25 RPM	26.3	2	1.3	Pass	
	Pass				

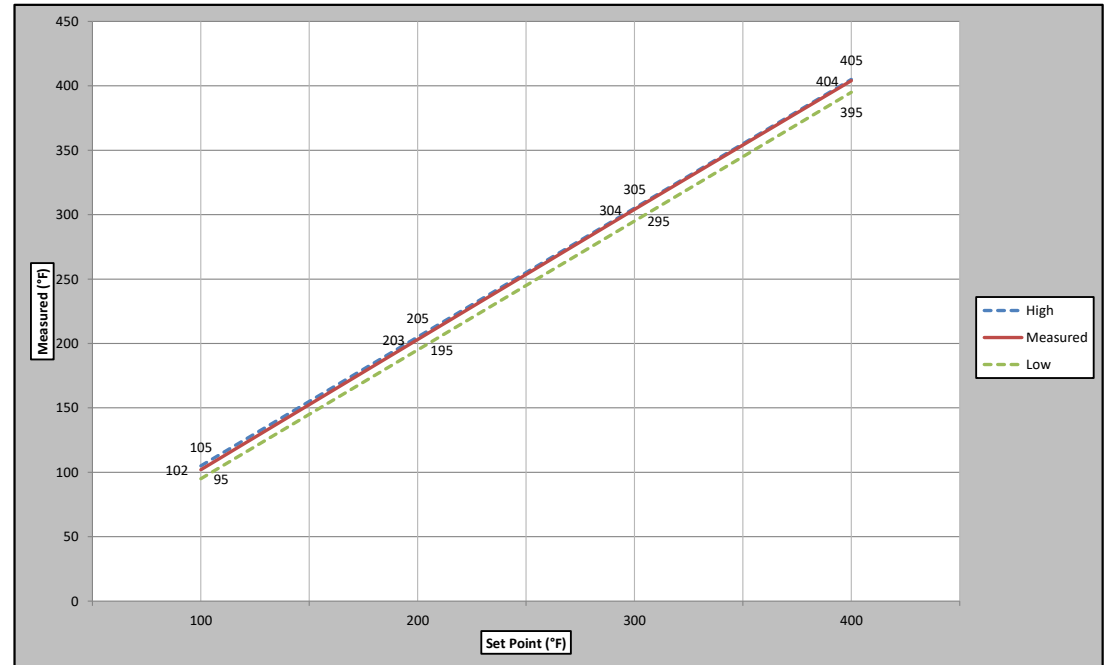

Calibration Technician: Shawn Maglitto

Technician Signature: *Shawn Maglitto*

Date: 12/9/2025

Reviewed By: Samantha Korenek

Reviewer Signature: *Samantha Korenek*

Review Date: 12/10/2025