



Dependable Products From People You Trust

# OFI TESTING EQUIPMENT, INC.

11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com


## CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

AS FOUND CHART

AS LEFT CHART

LAB TEMPERATURE	LAB HUMIDITY	PART NUMBER	SERIAL NUMBER	SET POINT	RESULT	ALLOWABLE RANGE	CALIBRATION DATE	DUE DATE	TECHNICIAN
58.00 °F	33.00 %	165-14-2	5079280000004	930.0 °F	916.5 °F	860-1000 °F	11/20/2024	11/20/2025	SM

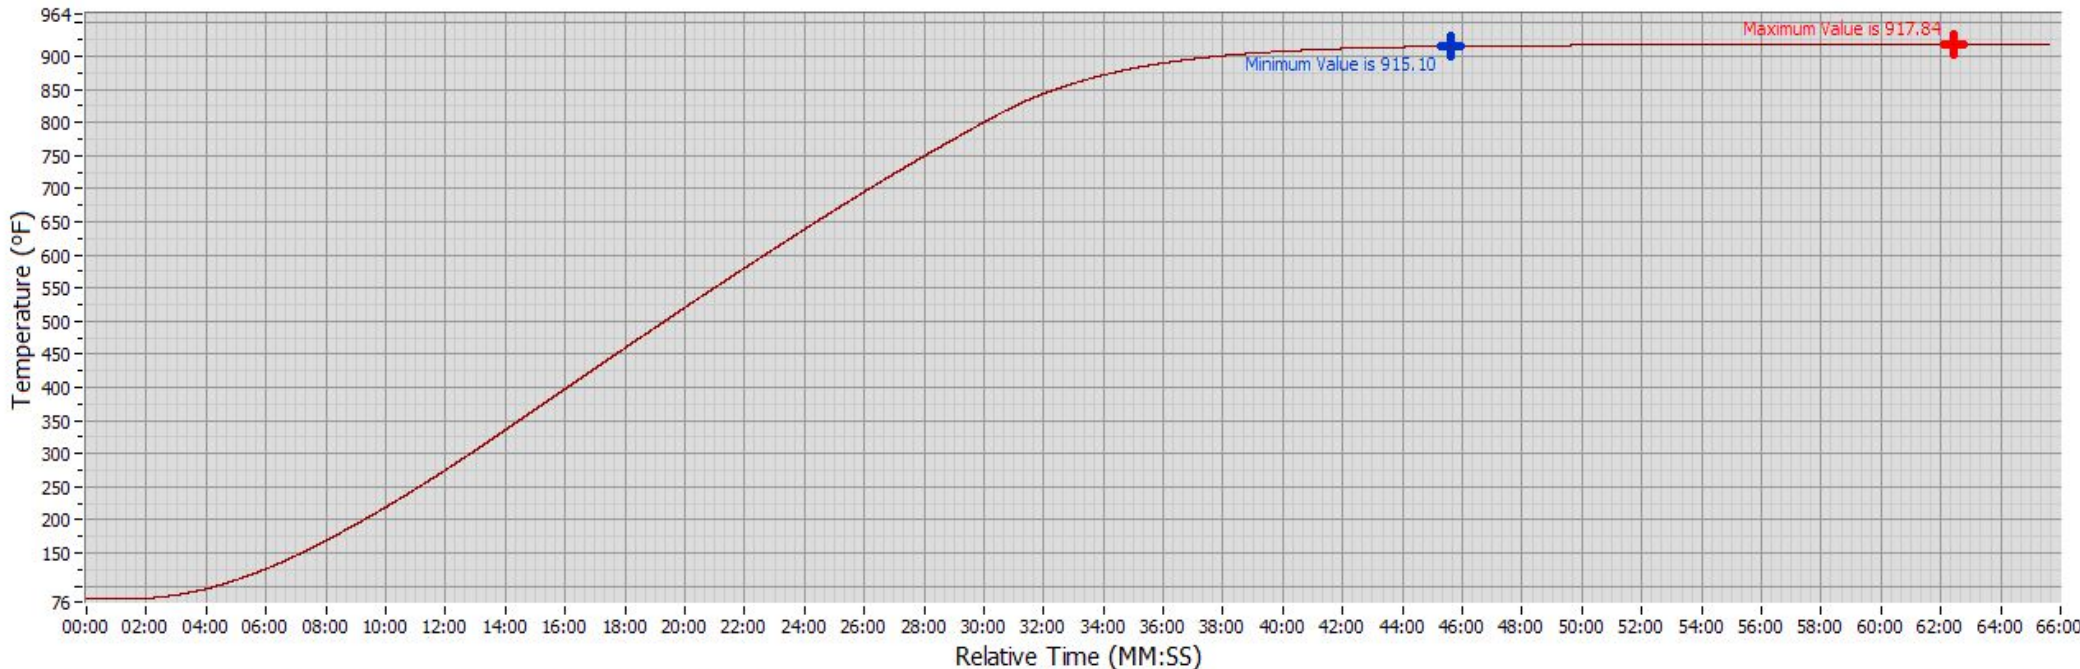

Calibration station has been calibrated using instruments which are traceable to NIST.

**CAL STATION SERIAL NUMBER:** 6B-11     
**CAL STATION CALIBRATION DATE:** 11/11/2024     
**CAL STATION DUE DATE:** 11/11/2025  
**AMBIENT MONITOR MODEL:** RH101     
**AMBIENT MONITOR S/N:** Z375174     
**AMBIENT MONITOR CAL DATE:** 01/16/2024     
**AMBIENT MONITOR DUE DATE:** 01/16/2025  
**UNCERTAINTY:** ± 2.8°C / 5°F     
**CALIBRATION PROCEDURE USED:** Retort Calibration Procedures API RP 13B-1

- Channel 5
- Plot 1
- Plot 2
- Plot 3
- Plot 4

**AS FOUND CONDITION:**

**CALIBRATION RESULT:** Accepted