



Dependable Products From People You Trust

# OFI TESTING EQUIPMENT, INC.


11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com

## CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

- AS FOUND CHART
- AS LEFT CHART

<b>LAB TEMPERATURE</b> 65.00 °F	<b>LAB HUMIDITY</b> 60.00 %	<b>PART NUMBER</b> 165-14-1	<b>SERIAL NUMBER</b> 5374970000007	<b>SET POINT</b> 930.0 °F	<b>RESULT</b> 960.9 °F	<b>ALLOWABLE RANGE</b> 860-1000 °F	<b>CALIBRATION DATE</b> 12/18/2024	<b>DUE DATE</b> 12/18/2025	<b>TECHNICIAN</b> SM
------------------------------------	--------------------------------	--------------------------------	---------------------------------------	------------------------------	---------------------------	---------------------------------------	---------------------------------------	-------------------------------	-------------------------

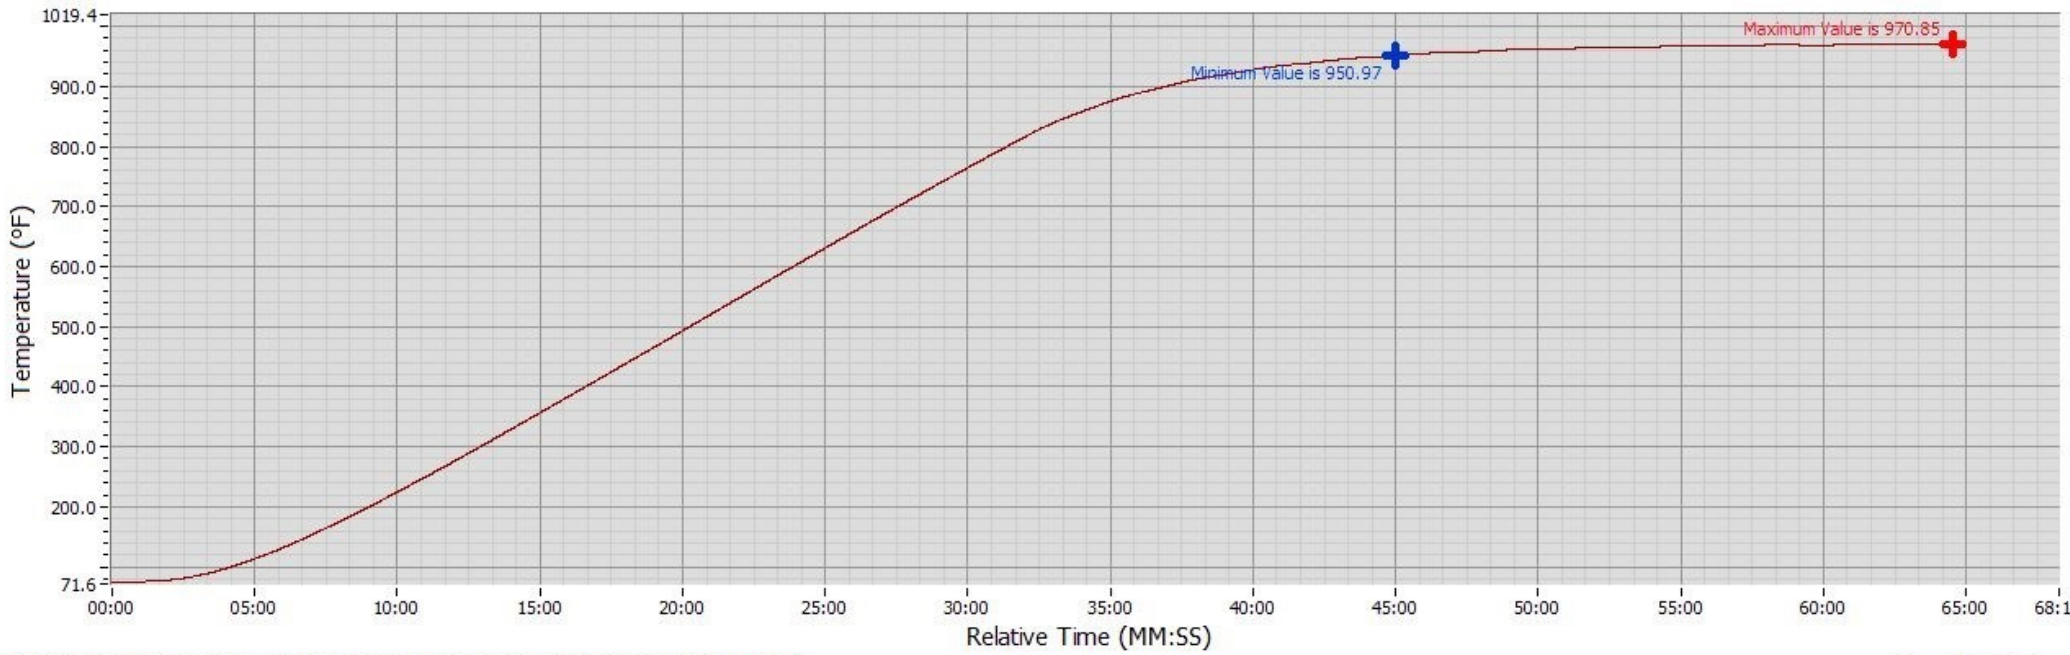

Calibration station has been calibrated using instruments which are traceable to NIST.

**CAL STATION SERIAL NUMBER:** 6B-11   
**CAL STATION CALIBRATION DATE:** 11/11/2024   
**CAL STATION DUE DATE:** 11/11/2025  
**AMBIENT MONITOR MODEL:** RH101   
**AMBIENT MONITOR S/N:** Z375174   
**AMBIENT MONITOR CAL DATE:** 01/16/2024   
**AMBIENT MONITOR DUE DATE:** 01/16/2025  
**UNCERTAINTY:** ± 2.8°C / 5°F   
**CALIBRATION PROCEDURE USED:** Retort Calibration Procedures API RP 13B-1

**AS FOUND CONDITION:**

**CALIBRATION RESULT:** Accepted