



Dependable Products From People You Trust

# OFI TESTING EQUIPMENT, INC.


11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com

## CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

- AS FOUND CHART
- AS LEFT CHART

LAB TEMPERATURE	LAB HUMIDITY	PART NUMBER	SERIAL NUMBER	SET POINT	RESULT	ALLOWABLE RANGE	CALIBRATION DATE	DUE DATE	TECHNICIAN
59.00 °F	43.00 %	165-14-1	537844000006	930.0 °F	976.3 °F	860-1000 °F	12/19/2024	12/19/2025	SM

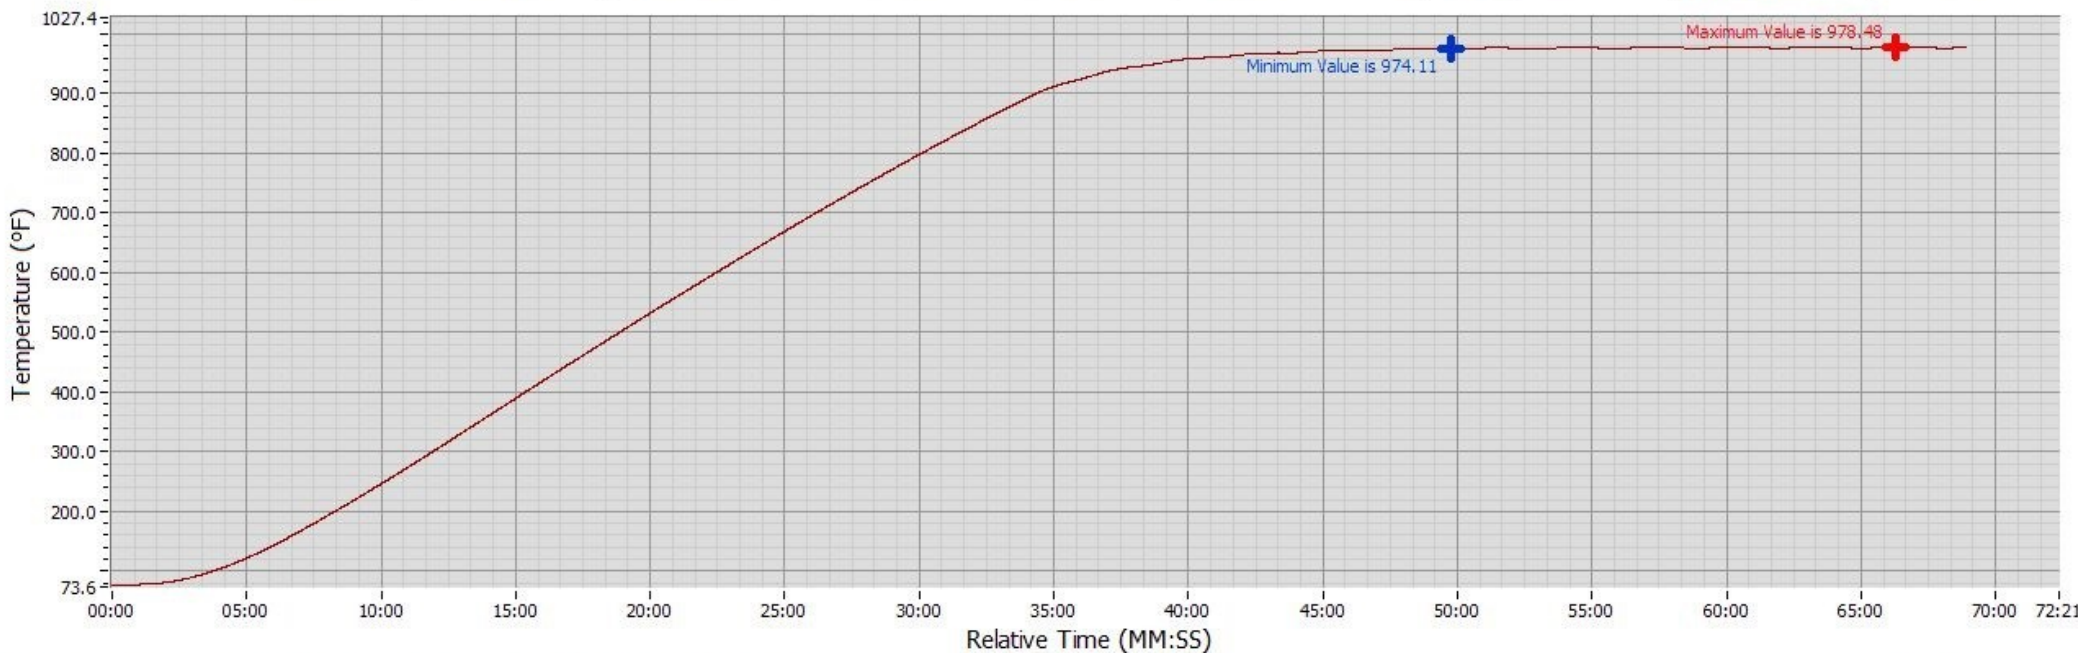

Calibration station has been calibrated using instruments which are traceable to NIST.

Channel 6

**CAL STATION SERIAL NUMBER:** 6B-11   
**CAL STATION CALIBRATION DATE:** 11/11/2024   
**CAL STATION DUE DATE:** 11/11/2025  
**AMBIENT MONITOR MODEL:** RH101   
**AMBIENT MONITOR S/N:** Z375174   
**AMBIENT MONITOR CAL DATE:** 01/16/2024   
**AMBIENT MONITOR DUE DATE:** 01/16/2025  
**UNCERTAINTY:** ± 2.8°C / 5°F   
**CALIBRATION PROCEDURE USED:** Retort Calibration Procedures API RP 13B-1

**AS FOUND CONDITION:**

**CALIBRATION RESULT:** Accepted