



Dependable Products From People You Trust

OFI TESTING EQUIPMENT, INC.

11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com


CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

AS FOUND CHART

AS LEFT CHART

LAB TEMPERATURE 59.00 °F	LAB HUMIDITY 43.00 %	PART NUMBER 165-14-1	SERIAL NUMBER 5378440000010	SET POINT 930.0 °F	RESULT 942.6 °F	ALLOWABLE RANGE 860-1000 °F	CALIBRATION DATE 12/19/2024	DUE DATE 12/19/2025	TECHNICIAN SM
------------------------------------	--------------------------------	--------------------------------	---------------------------------------	------------------------------	---------------------------	---------------------------------------	---------------------------------------	-------------------------------	-------------------------

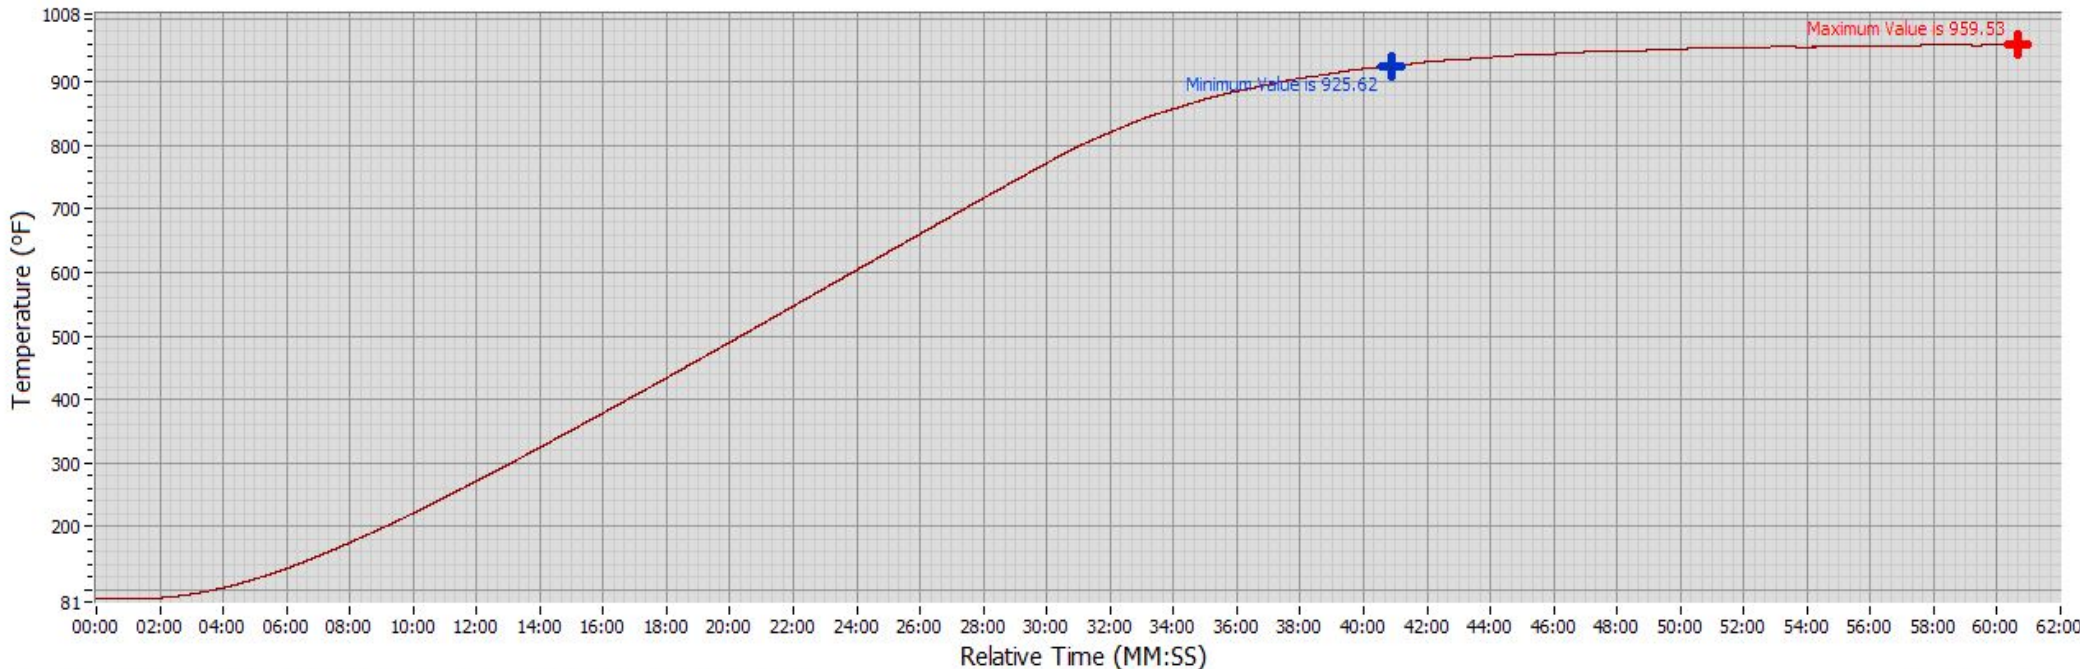

Calibration station has been calibrated using instruments which are traceable to NIST.

CAL STATION SERIAL NUMBER: 6B-11	CAL STATION CALIBRATION DATE: 11/11/2024	CAL STATION DUE DATE: 11/11/2025
AMBIENT MONITOR MODEL: RH101	AMBIENT MONITOR S/N: Z375174	AMBIENT MONITOR CAL DATE: 01/16/2024 AMBIENT MONITOR DUE DATE: 01/16/2025
UNCERTAINTY: ± 2.8°C / 5°F	CALIBRATION PROCEDURE USED: Retort Calibration Procedures API RP 13B-1	

- Channel 10
- Plot 1
- Plot 2
- Plot 3
- Plot 4

AS FOUND CONDITION:

CALIBRATION RESULT: Accepted