



Dependable Products From People You Trust

# OFI TESTING EQUIPMENT, INC.

11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com


## CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

AS FOUND CHART

AS LEFT CHART

<b>LAB TEMPERATURE</b> 59.00 °F	<b>LAB HUMIDITY</b> 43.00 %	<b>PART NUMBER</b> 165-14-3-LR	<b>SERIAL NUMBER</b> 5377540000003	<b>SET POINT</b> 930.0 °F	<b>RESULT</b> 897.9 °F	<b>ALLOWABLE RANGE</b> 860-1000 °F	<b>CALIBRATION DATE</b> 12/23/2024	<b>DUE DATE</b> 12/23/2025	<b>TECHNICIAN</b> SM
------------------------------------	--------------------------------	-----------------------------------	---------------------------------------	------------------------------	---------------------------	---------------------------------------	---------------------------------------	-------------------------------	-------------------------

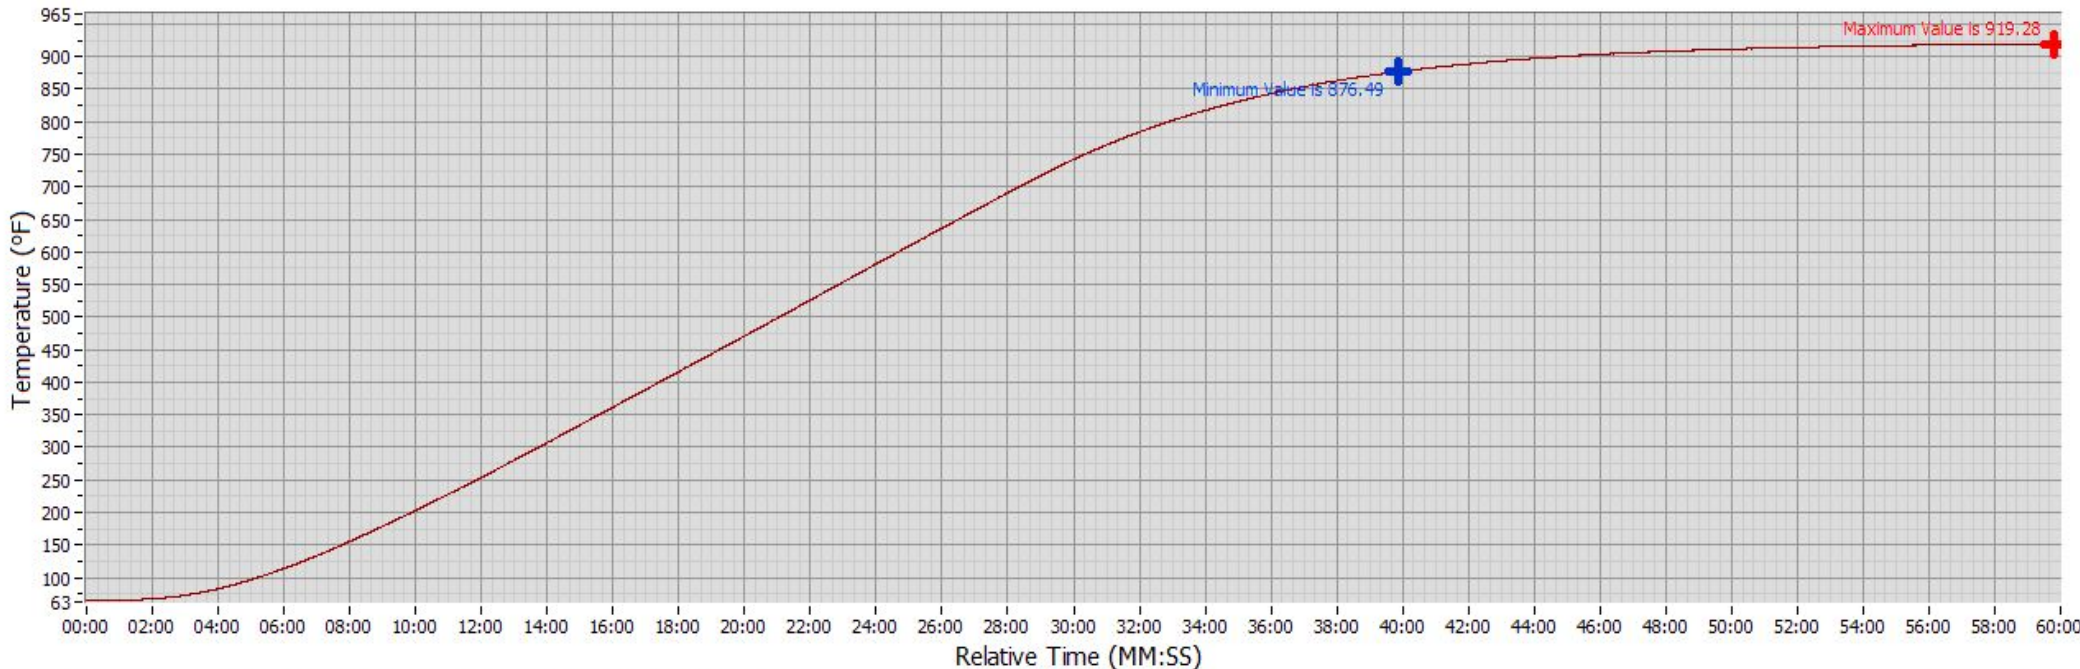

Calibration station has been calibrated using instruments which are traceable to NIST.

<b>CAL STATION SERIAL NUMBER:</b> 6B-11	<b>CAL STATION CALIBRATION DATE:</b> 11/11/2024	<b>CAL STATION DUE DATE:</b> 11/11/2025
<b>AMBIENT MONITOR MODEL:</b> RH101	<b>AMBIENT MONITOR S/N:</b> Z375174	<b>AMBIENT MONITOR CAL DATE:</b> 01/16/2024 <b>AMBIENT MONITOR DUE DATE:</b> 01/16/2025
<b>UNCERTAINTY:</b> ± 2.8°C / 5°F	<b>CALIBRATION PROCEDURE USED:</b> Retort Calibration Procedures API RP 13B-1	

- Channel 3
- Plot 1
- Plot 2
- Plot 3
- Plot 4

**AS FOUND CONDITION:**

**CALIBRATION RESULT:** Accepted