



OFI Testing Equipment, Inc.
 11302 Steeplecrest Drive Houston, TX 77065 USA
 Phone: 832-320-7300 · Fax: 713-880-9886 · Web: www.ofite.com


Roller Oven Series Calibration Report

Repairs Required? No As Found Data Required by Customer? No Static Oven: No (°F) or (°C): (°F) Max Temp: 500
 Part Number: 172-00-1-C Manufacturer: OFI Testing Equipment Serial Number: 5377060000001 S/O# or W/O# NEW

Master Testing Equipment
 Thermometer: 154 Model #: EA10 Serial #: Z375331 Calibration Due: 7/24/2025 Tachometer: 678 Model #: R7050 Serial #: 220326760 Calibration Due: 7/22/2025

Ambient Conditions
 Ambient Monitor: 345 Model No: RH300 Calibration Date: 8/20/2024 Calibration Due: 8/20/2025 Serial No: Z395285
 Ambient Conditions: Room Temperature: 66 Relative Humidity: 60.0%

AS LEFT MEASUREMENTS		(°F)	Max Oven Temp	500	
Set point	Process Temperature	Accepted Deviation	Actual Deviation	Pass/Fail	
100	100	5	0	Pass	
200	203	5	3	Pass	
300	303	5	3	Pass	
400	404	5	4	Pass	
500	500	5	0	Pass	
25 RPM	24.8	2	-0.2	Pass	
				Pass	

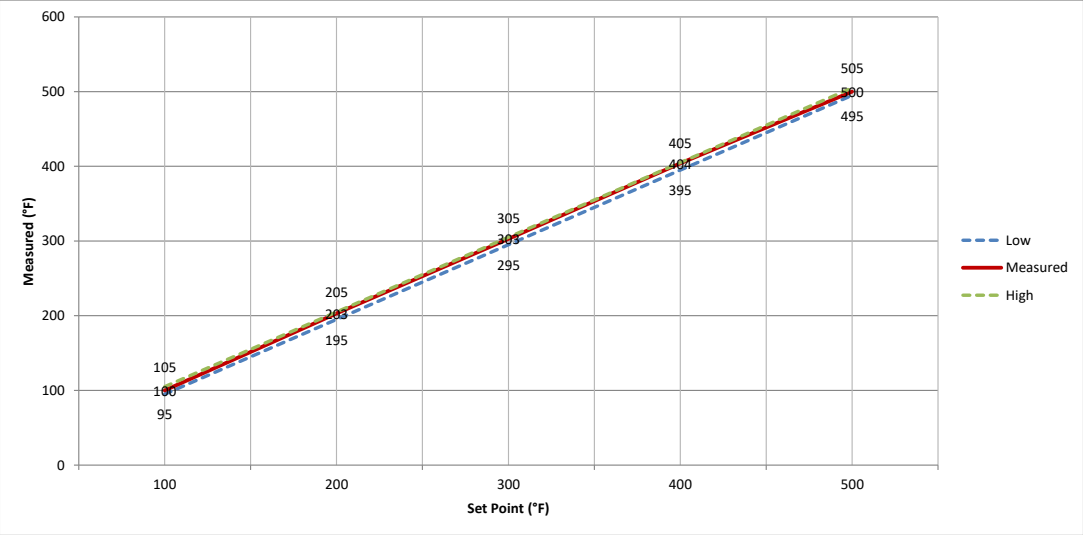

Technician: Shawn Maglitto
 Calibration Date: 12/26/2024
 Recommended Calibration Date *: 12/26/2025
 * To be provided by customer
 Reviewed By: Samantha Korenek
 Review Date: 12/26/2024