



Dependable Products From People You Trust

# OFI TESTING EQUIPMENT, INC.

11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com


## CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

AS FOUND CHART

AS LEFT CHART

| LAB TEMPERATURE | LAB HUMIDITY | PART NUMBER | SERIAL NUMBER | SET POINT | RESULT   | ALLOWABLE RANGE | CALIBRATION DATE | DUE DATE   | TECHNICIAN |
|-----------------|--------------|-------------|---------------|-----------|----------|-----------------|------------------|------------|------------|
| 66.00 °F        | 60.00 %      | 165-14      | 5375090000009 | 930.0 °F  | 966.9 °F | 860-1000 °F     | 12/26/2024       | 12/26/2025 | SM         |

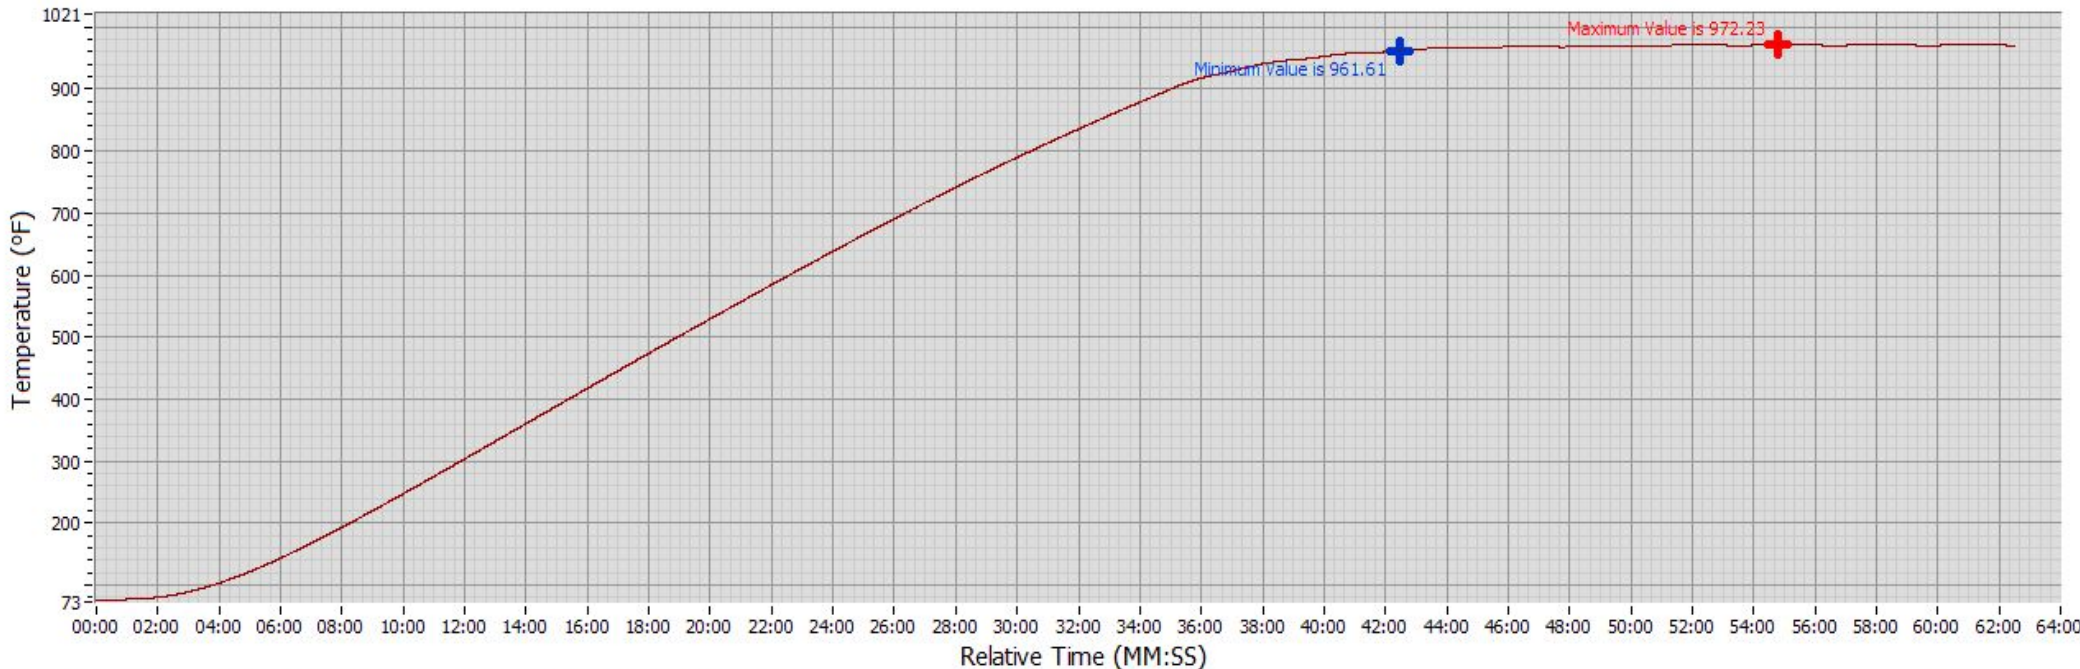

Calibration station has been calibrated using instruments which are traceable to NIST.

**CAL STATION SERIAL NUMBER:** 6B-11      **CAL STATION CALIBRATION DATE:** 11/11/2024      **CAL STATION DUE DATE:** 11/11/2025

**AMBIENT MONITOR MODEL:** RH101      **AMBIENT MONITOR S/N:** Z375174      **AMBIENT MONITOR CAL DATE:** 01/16/2024      **AMBIENT MONITOR DUE DATE:** 01/16/2025

**UNCERTAINTY:** ± 2.8°C / 5°F      **CALIBRATION PROCEDURE USED:** Retort Calibration Procedures API RP 13B-1

- Channel 9
- Plot 1
- Plot 2
- Plot 3
- Plot 4

**AS FOUND CONDITION:**

**CALIBRATION RESULT:** Accepted