



OFI Testing Equipment, Inc.
 11302 Steeplecrest Drive Houston, TX 77065 USA
 Phone: 832-320-7300 · Fax: 713-880-9886 · Web: www.ofite.com


Roller Oven Series Calibration Report

Repairs Required? Yes (See damage report below) As Found Data Required by Customer? No Static Oven: No (°F) or (°C): (°F) Max Temp: 400
 Part Number: 173-00-RC Manufacturer: OFI Testing Equipment Serial Number: 501761000001 S/O# or W/O# 0022358

Master Testing Equipment
 Thermometer: 257 Model #: EA10 Serial #: Z375329 Calibration Due: 2/17/2025 Tachometer: 710 Model #: 461920 Serial #: 131105873 Calibration Due: 5/8/2025

Ambient Conditions
 Ambient Monitor: 345 Model No: RH300 Calibration Date: 8/20/2024 Calibration Due: 8/20/2025 Serial No: Z395285
 Ambient Conditions: Room Temperature: 61 Relative Humidity: 48.0%

| AS LEFT MEASUREMENTS | | (°F) | Max Oven Temp | 400 | |
|----------------------|---------------------|--------------------|------------------|-----------|--|
| Set point | Process Temperature | Accepted Deviation | Actual Deviation | Pass/Fail | |
| 100 | 100 | 5 | 0 | Pass | |
| 200 | 199 | 5 | -1 | Pass | |
| 300 | 301 | 5 | 1 | Pass | |
| 400 | 403 | 5 | 3 | Pass | |
| 25 RPM | 24.3 | 2 | -0.7 | Pass | |
| | | | | Pass | |

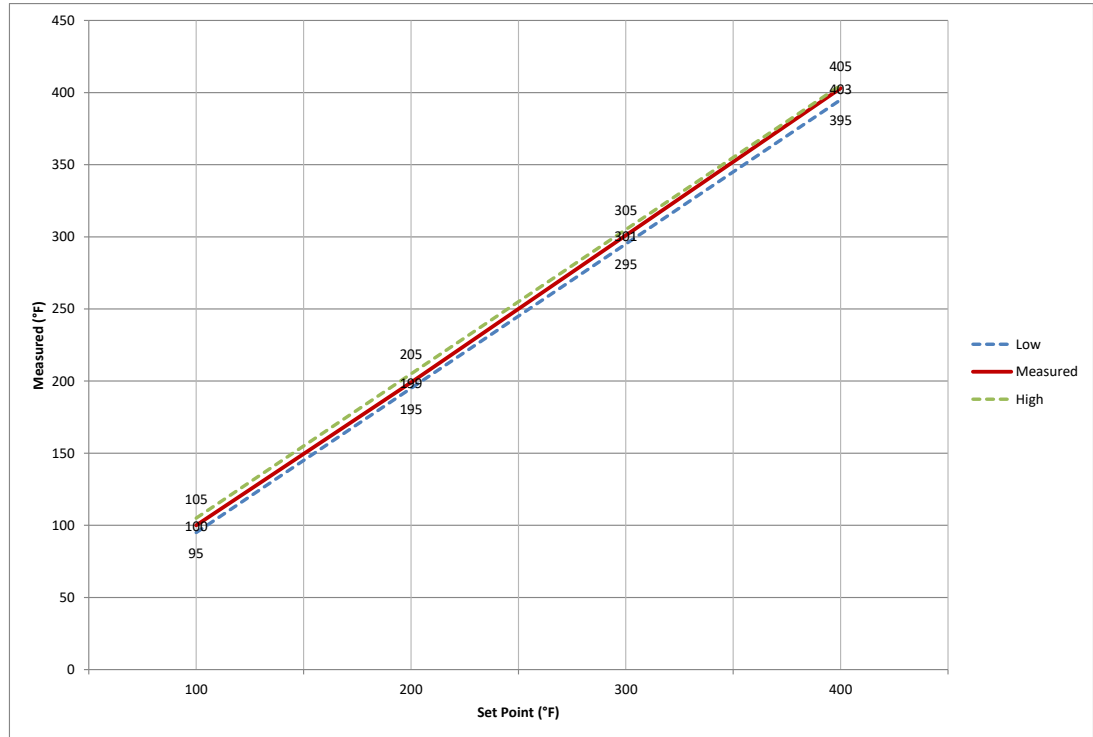

Technician: Shawn Maglitto
 Calibration Date: 12/23/2024
 Recommended Calibration Date *: 12/23/2025
 * To be provided by customer
 Reviewed By: Samantha Korenek
 Review Date: 12/23/2024

Damage Report

List all damages. Describe how this could have affected measurements.

List all repairs made prior to AS LEFT measurements.

This report meets or exceeds the requirements outlined in API RP 13B-1 Recommended Practice for Field Testing Water-based Drilling Fluids and API RP 13B-2 Recommended Practice for Field Testing Oil-based Drilling Fluids for calibration of laboratory devices, using certified master test equipment that is traceable to NIST.