



Dependable Products From People You Trust

OFI TESTING EQUIPMENT, INC.

11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com


CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

AS FOUND CHART

AS LEFT CHART

LAB TEMPERATURE 59.00 °F	LAB HUMIDITY 42.00 %	PART NUMBER 165-14-3	SERIAL NUMBER 5376740000002	SET POINT 930.0 °F	RESULT 902.6 °F	ALLOWABLE RANGE 860-1000 °F	CALIBRATION DATE 1/2/2025	DUE DATE 1/2/2026	TECHNICIAN SM
------------------------------------	--------------------------------	--------------------------------	---------------------------------------	------------------------------	---------------------------	---------------------------------------	-------------------------------------	-----------------------------	-------------------------

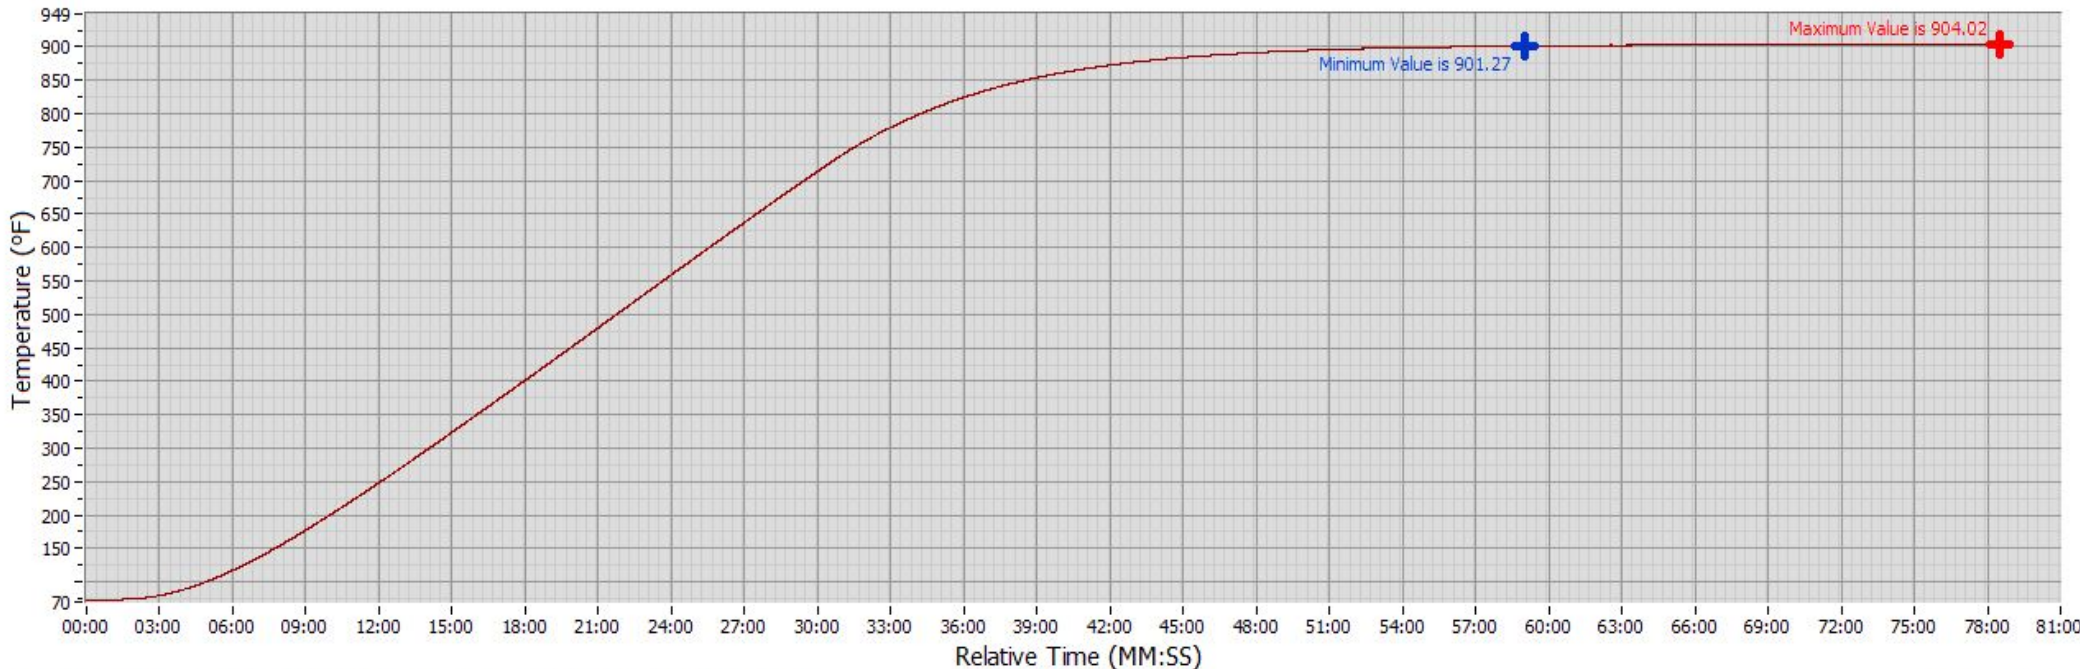

Calibration station has been calibrated using instruments which are traceable to NIST.

CAL STATION SERIAL NUMBER: 6B-11 **CAL STATION CALIBRATION DATE:** 11/11/2024 **CAL STATION DUE DATE:** 11/11/2025

AMBIENT MONITOR MODEL: RH101 **AMBIENT MONITOR S/N:** Z375174 **AMBIENT MONITOR CAL DATE:** 01/16/2024 **AMBIENT MONITOR DUE DATE:** 01/16/2025

UNCERTAINTY: ± 2.8°C / 5°F **CALIBRATION PROCEDURE USED:** Retort Calibration Procedures API RP 13B-1

- Channel 2
- Plot 1
- Plot 2
- Plot 3
- Plot 4

AS FOUND CONDITION:

CALIBRATION RESULT: Accepted