



**OFI Testing Equipment, Inc.**  
 11302 Steeplecrest Drive Houston, TX 77065 USA  
 Phone: 832-320-7300 · Fax: 713-880-9886 · Web: www.ofite.com


**Roller Oven Series Calibration Report**

Repairs Required? No As Found Data Required by Customer? No Static Oven: No (°F) or (°C): (°F) Max Temp: 500  
 Part Number: 173-00-1-C Manufacturer: OFI Testing Equipment Serial Number: 5375940000001 S/O# or W/O# NEW

**Master Testing Equipment**  
 Thermometer: 257 Model #: EA10 Serial #: Z375329 Calibration Due: 2/17/2025 Tachometer: 708 Model #: R7050 Serial #: Z30832873 Calibration Due: 1/30/2025

**Ambient Conditions**  
 Ambient Monitor: 345 Model No: RH300 Calibration Date: 8/20/2024 Calibration Due: 8/20/2025 Serial No: Z395285  
 Ambient Conditions: Room Temperature: 61 Relative Humidity: 50.0%

AS LEFT MEASUREMENTS		(°F)	Max Oven Temp	500	
Set point	Process Temperature	Accepted Deviation	Actual Deviation	Pass/Fail	
100	96	5	-4	Pass	
200	202	5	2	Pass	
300	303	5	3	Pass	
400	401	5	1	Pass	
500	499	5	-1	Pass	
25 RPM	24.5	2	-0.5	Pass	
				Pass	

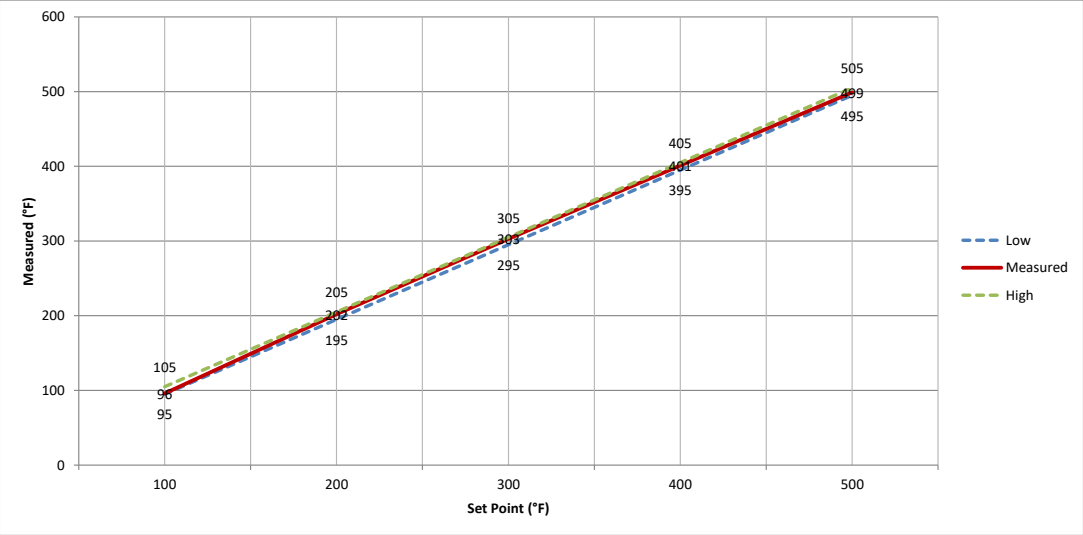

Technician: Shawn Maglitto  
 Calibration Date: 1/3/2025  
 Recommended Calibration Date \*: 1/3/2026  
 \* To be provided by customer  
 Reviewed By: Samantha Korenek  
 Review Date: 1/6/2025