



OFI Testing Equipment, Inc.
 11302 Steeplecrest Drive Houston, TX 77065 USA
 Phone: 832-320-7300 · Fax: 713-880-9886 · Web: www.ofite.com

176-00 Roller Oven Calibration Report

Repairs Required? No

As Found Data Required by Customer? No

Static Oven: No

(°F) or (°C) : (°F)

Part Number: 176-00-C

Manufacturer: OFI Testing Equipment

Serial Number: 5376570000001

S/O# or J/O# NEW


Master Testing Equipment

Thermometer: 336 Model #: EA10 Serial #: 171103418 Calibration Due: 8/22/2025 Tachometer: 710 Model #: 461920 Serial #: 131105873 Calibration Due: 5/8/2025

Ambient Conditions

Ambient Monitor: 345 Model No: RH300 Calibration Date: 8/20/2024 Calibration Due: 8/20/2025 Serial No: Z395285
 Ambient Conditions: Room Temperature: 57 Relative Humidity: 41

AS LEFT MEASUREMENTS		°F		
Set point	Process Temperature	Accepted Deviation	Actual Deviation	Pass/Fail
100	99	5	-1	Pass
200	201	5	1	Pass
300	304	5	4	Pass
400	404	5	4	Pass
500	499	5	-1	Pass
600	596	5	-4	Pass
25 RPM	24.7	2	-0.3	Pass
				Pass

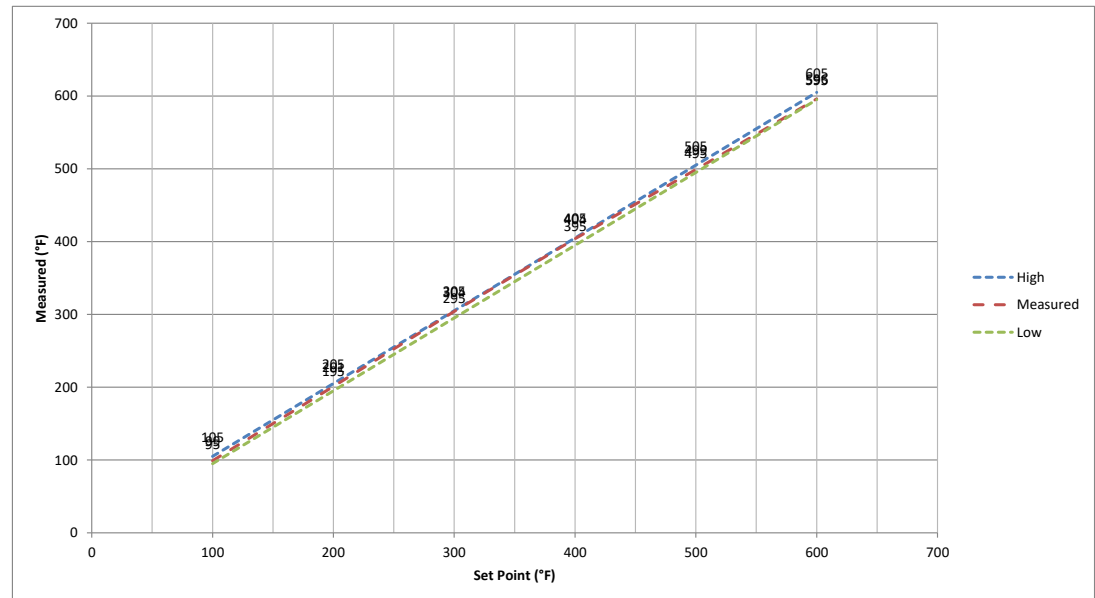

Technician: Shawn Maglitto

Calibration Date: 1/17/2025

Recommended Calibration Date *: 1/17/2026

* To be provided by customer

Reviewed By: Samantha Korenek

Review Date: 1/17/2025

This report meets or exceeds the requirements outlined in API RP 13B-1 Recommended Practice for Field Testing Water-based Drilling Fluids and API RP 13B-2 Recommended Practice for Field Testing Oil-based Drilling Fluids for calibration of laboratory devices, using certified master test equipment that is traceable to NIST.