



Dependable Products From People You Trust

OFI TESTING EQUIPMENT, INC.

11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com


CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

AS FOUND CHART

AS LEFT CHART

LAB TEMPERATURE 66.00 °F	LAB HUMIDITY 72.00 %	PART NUMBER 165-14-1	SERIAL NUMBER 5378450000002	SET POINT 930.0 °F	RESULT 973.1 °F	ALLOWABLE RANGE 860-1000 °F	CALIBRATION DATE 1/30/2025	DUE DATE 1/30/2026	TECHNICIAN SM
------------------------------------	--------------------------------	--------------------------------	---------------------------------------	------------------------------	---------------------------	---------------------------------------	--------------------------------------	------------------------------	-------------------------

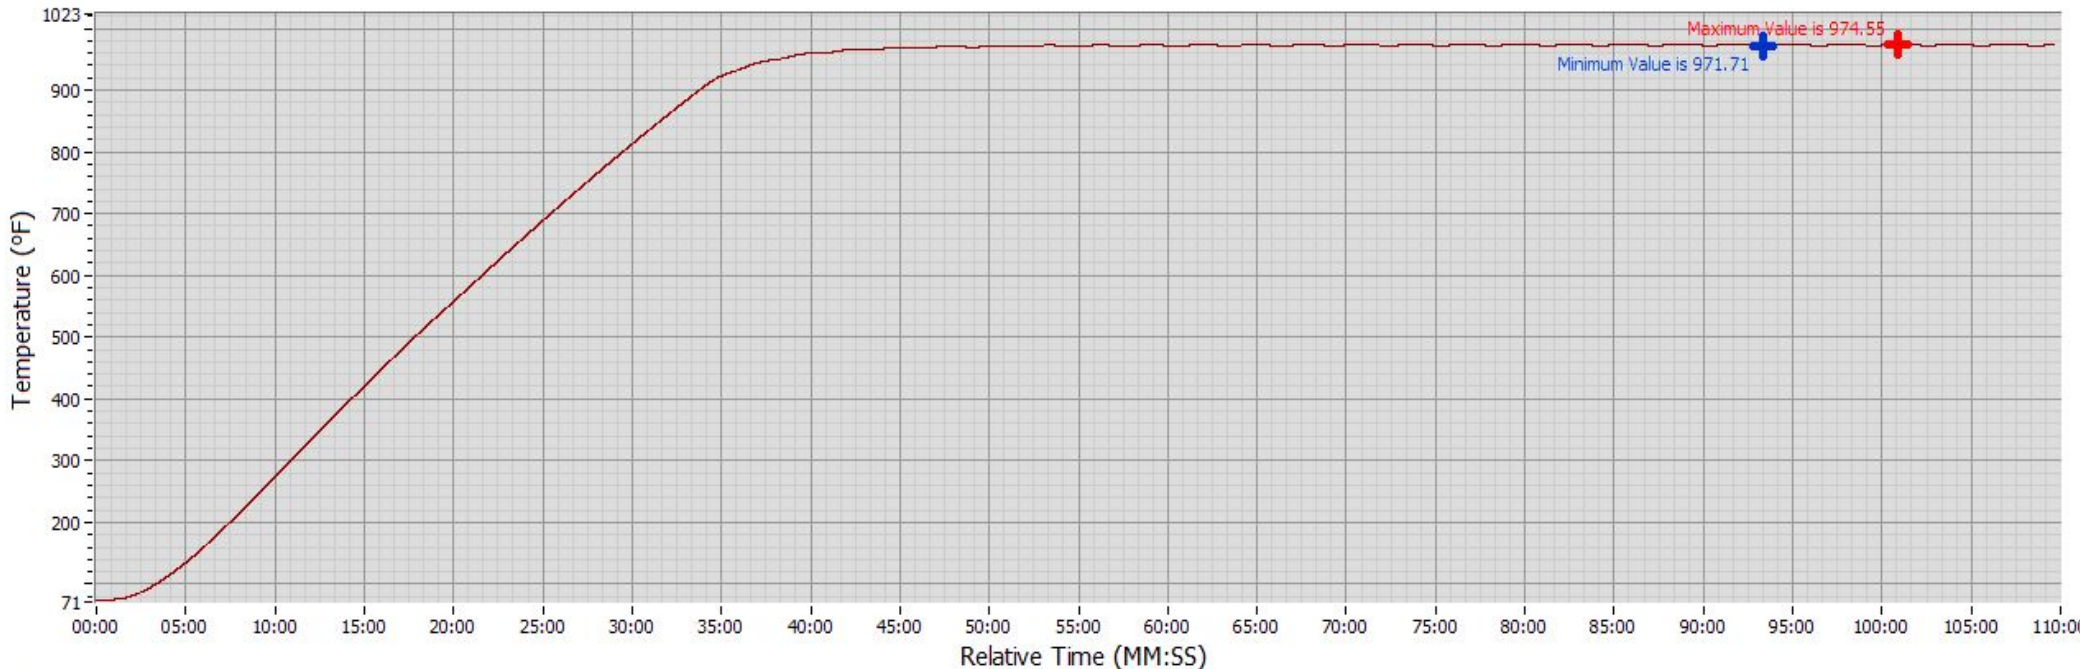

Calibration station has been calibrated using instruments which are traceable to NIST.

CAL STATION SERIAL NUMBER: 6B-11	CAL STATION CALIBRATION DATE: 11/11/2024	CAL STATION DUE DATE: 11/11/2025
AMBIENT MONITOR MODEL: RH300	AMBIENT MONITOR S/N: Z395285	AMBIENT MONITOR CAL DATE: 08/20/2024 AMBIENT MONITOR DUE DATE: 08/20/2025
UNCERTAINTY: ± 2.8°C / 5°F	CALIBRATION PROCEDURE USED: Retort Calibration Procedures API RP 13B-1	

- Channel 2
- Plot 1
- Plot 2
- Plot 3
- Plot 4

AS FOUND CONDITION:

CALIBRATION RESULT: Accepted