



Roller Oven Calibration Report


Order Number:	22467
Serial # / Local I.D. #:	5915
Calibration Date:	2/28/2025
Recommended Due Date:	2/28/2026
Certificate Number:	591545716
Manufacturer:	OFI Testing Equipment
Part Number:	174-00

Condition Found:	NEW
Condition Left:	In Calibration
Repairs Required:	No
Static Oven:	No
(F) or (C):	(°F)
Max Temp:	400
As Found Required:	No

OFI Testing Equipment, Inc. - 11302 Steeplecrest Dr - Houston, Texas - 77065 - Phone: 832.320.7300 - Web: www.ofite.com

Calibration Equipment						
Thermometer	336	EA10	171103418	C-40409	8/22/2024	8/22/2025
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Tachometer	679	R7050	220326766	38254	7/22/2024	7/22/2025
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Ambient Monitor	345	RH300	Z395285	C-40456	8/20/2024	8/20/2025
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Ambient Conditions	Lab / Room Temperature		59.5	(°F)	Lab / Room Humidity	
						42.1 %

AS LEFT MEASUREMENTS		(°F)	Max Oven Temp	400	
Set point	Process Temperature	Accepted Deviation	Actual Deviation	Pass/Fail	
100.0	102.0	5	2.0	Pass	
	Pass				
200.0	197.0	5	-3.0	Pass	
	Pass				
300.0	296.0	5	-4.0	Pass	
	Pass				
400.0	402.0	5	2.0	Pass	
	Pass				
25 RPM	23.8	2	-1.2	Pass	
	Pass				
					Pass

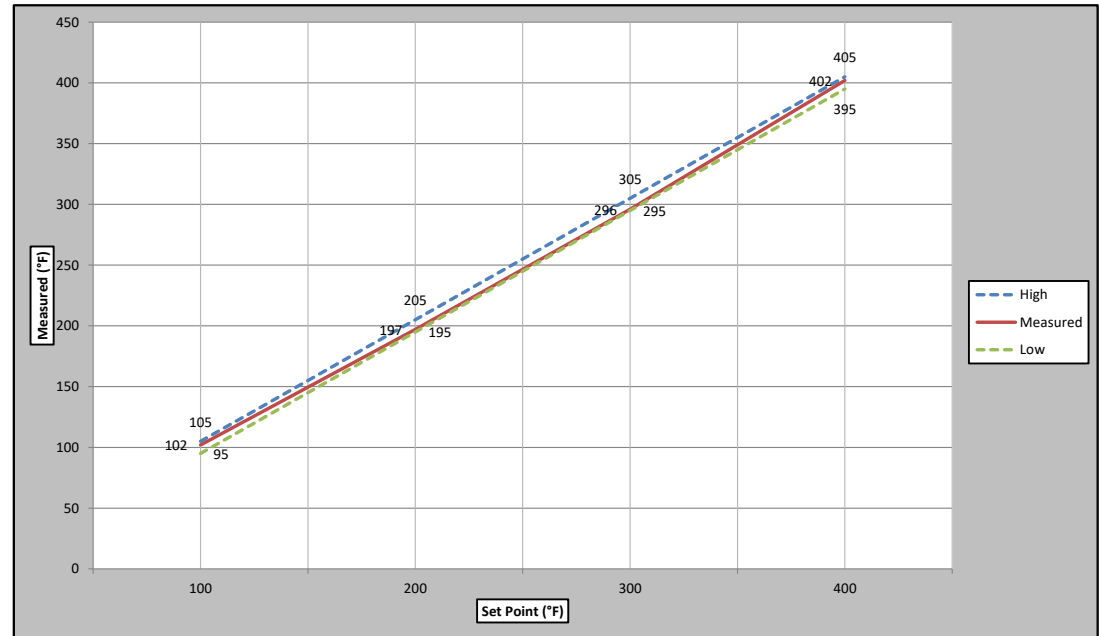

Calibration Technician: Shawn Maglitto

Date: 2/28/2025

Reviewed By: Samantha Korenek

Review Date: 3/4/2025