



Dependable Products From People You Trust

OFI TESTING EQUIPMENT, INC.

11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com


CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

AS FOUND CHART

AS LEFT CHART

| LAB TEMPERATURE | LAB HUMIDITY | PART NUMBER | SERIAL NUMBER | SET POINT | RESULT | ALLOWABLE RANGE | CALIBRATION DATE | DUE DATE | TECHNICIAN |
|-----------------|--------------|-------------|---------------|-----------|----------|-----------------|------------------|-----------|------------|
| 74.00 °F | 45.00 % | 165-14-3 | 5384890000008 | 930.0 °F | 927.0 °F | 860-1000 °F | 3/12/2025 | 3/12/2026 | SM |

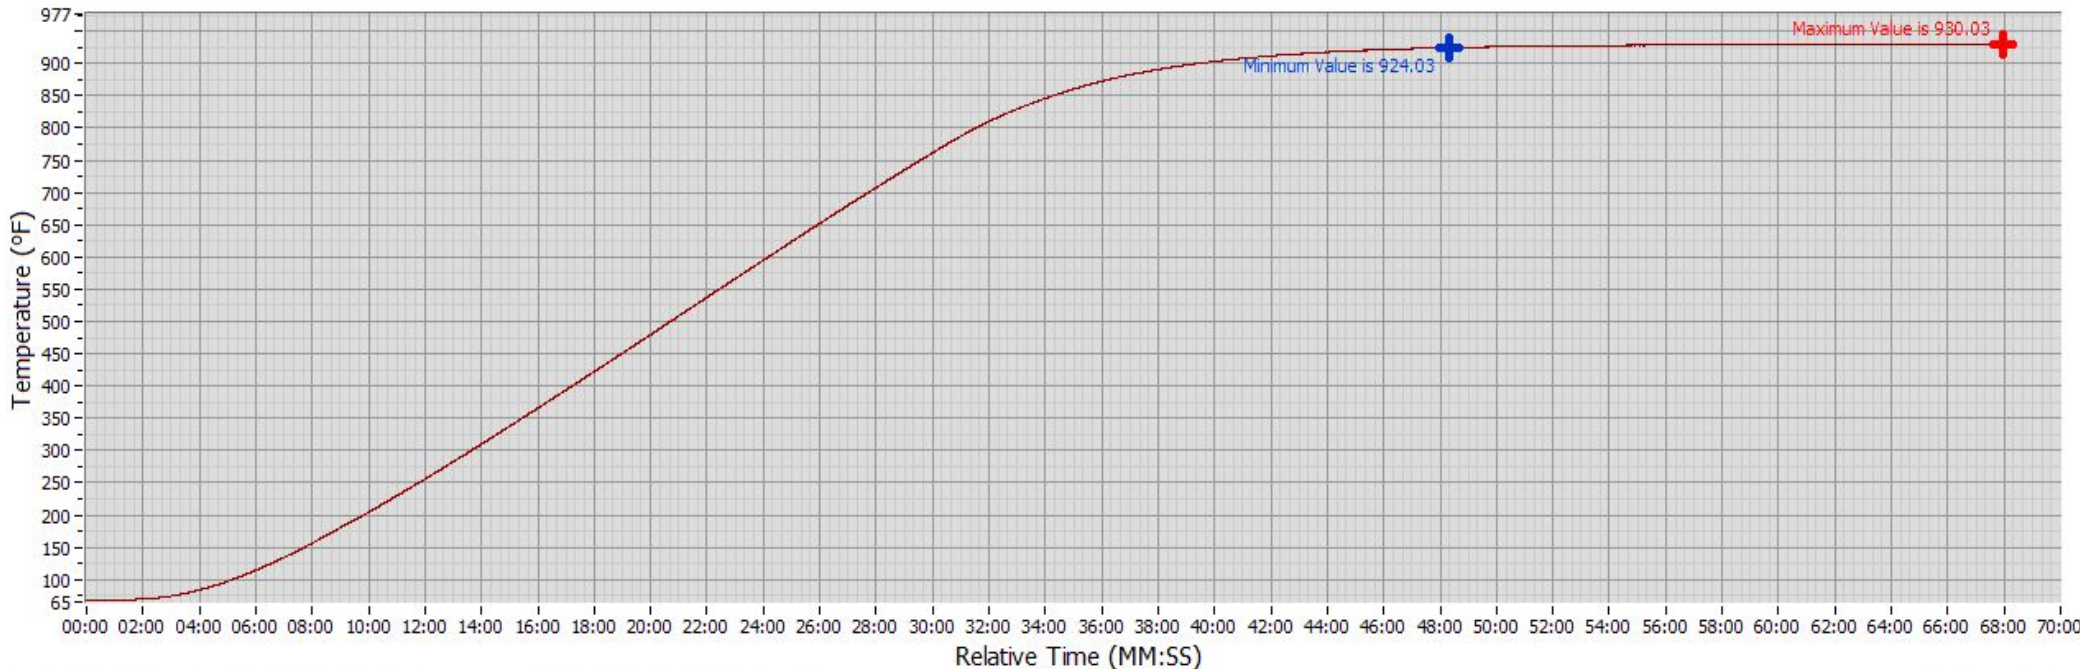

Calibration station has been calibrated using instruments which are traceable to NIST.

CAL STATION SERIAL NUMBER: 6B-11 **CAL STATION CALIBRATION DATE:** 11/11/2024 **CAL STATION DUE DATE:** 11/11/2025

AMBIENT MONITOR MODEL: RH300 **AMBIENT MONITOR S/N:** Z395285 **AMBIENT MONITOR CAL DATE:** 08/20/2024 **AMBIENT MONITOR DUE DATE:** 08/20/2025

UNCERTAINTY: ± 2.8°C / 5°F **CALIBRATION PROCEDURE USED:** Retort Calibration Procedures API RP 13B-1

- Channel 3
- Plot 1
- Plot 2
- Plot 3
- Plot 4

AS FOUND CONDITION:

CALIBRATION RESULT: Accepted