



Dependable Products From People You Trust

OFI TESTING EQUIPMENT, INC.

11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com


CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

AS FOUND CHART

AS LEFT CHART

LAB TEMPERATURE	LAB HUMIDITY	PART NUMBER	SERIAL NUMBER	SET POINT	RESULT	ALLOWABLE RANGE	CALIBRATION DATE	DUE DATE	TECHNICIAN
65.00 °F	58.00 %	170-01-1	5385380000004	375.0 °F	369.9 °F	350-400 °F	3/13/2025	3/13/2026	SM

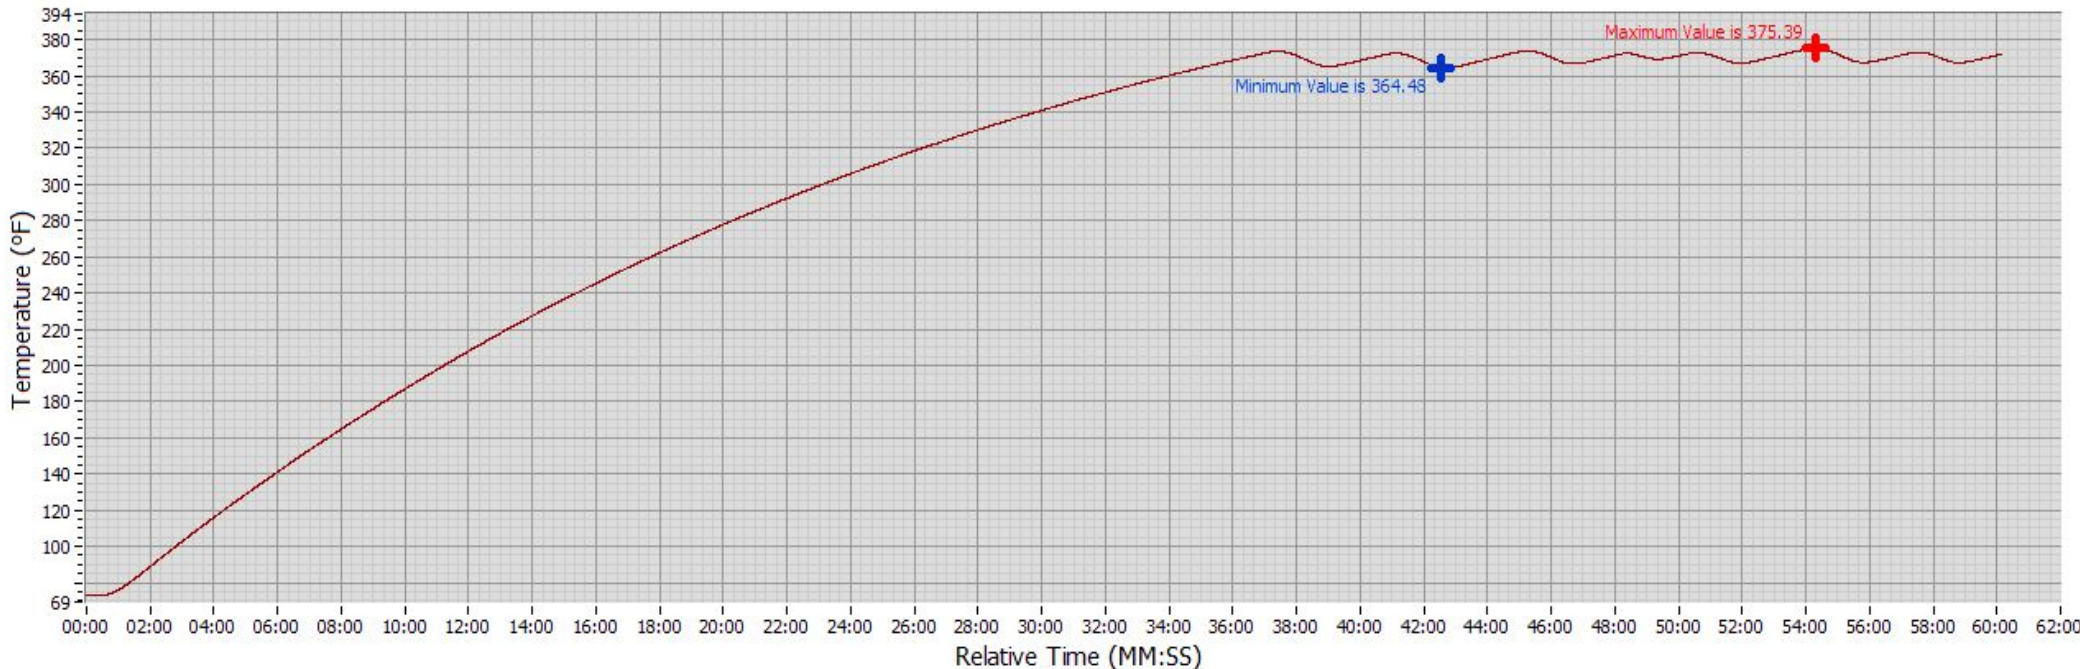

Calibration station has been calibrated using instruments which are traceable to NIST.

CAL STATION SERIAL NUMBER: 6B-11 **CAL STATION CALIBRATION DATE:** 11/11/2024 **CAL STATION DUE DATE:** 11/11/2025

AMBIENT MONITOR MODEL: RH300 **AMBIENT MONITOR S/N:** Z395285 **AMBIENT MONITOR CAL DATE:** 08/20/2024 **AMBIENT MONITOR DUE DATE:** 08/20/2025

UNCERTAINTY: ± 2.8°C / 5°F **CALIBRATION PROCEDURE USED:** 175 ml Heat Jacket Calibration Procedures API RP 13B-1

- Channel 4
- Plot 1
- Plot 2
- Plot 3
- Plot 4

AS FOUND CONDITION:

CALIBRATION RESULT: Accepted