



Roller Oven Calibration Report

Order Number:	22445
Serial # / Local I.D. #:	06-87
Calibration Date:	3/20/2025
Recommended Due Date:	3/20/2026
Certificate Number:	06-8745736
Manufacturer:	OFI Testing Equipment
Part Number:	173-00-C


Condition Found:	NEW
Condition Left:	In Calibration
Repairs Required:	Yes
Static Oven:	No
(F) or (C):	(°F)
Max Temp:	400
As Found Required:	No

OFI Testing Equipment, Inc. - 11302 Steeplecrest Dr - Houston, Texas - 77065 - Phone: 832.320.7300 - Web: www.ofite.com

Calibration Equipment						
Thermometer	336	EA10	171103418	C-40409	8/22/2024	8/22/2025
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Tachometer	710	461920	131105873	5-HZ7EP-120-1	5/8/2024	5/8/2025
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Ambient Monitor	345	RH300	Z395285	C-40456	8/20/2024	8/20/2025
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Ambient Conditions	Lab / Room Temperature		74.3	(°F)	Lab / Room Humidity	22.4 %

AS LEFT MEASUREMENTS		(°F)	Max Oven Temp	400	
Set point	Process Temperature	Accepted Deviation	Actual Deviation	Pass/Fail	
100.0	103.0	5	3.0	Pass	
	Pass				
200.0	203.0	5	3.0	Pass	
	Pass				
300.0	304.0	5	4.0	Pass	
	Pass				
400.0	400.0	5	0.0	Pass	
	Pass				
25 RPM	24.8	2	-0.2	Pass	
	Pass				
				Pass	

Calibration Technician: Shawn Maglitto
 Date: 3/20/2025
 Reviewed By: Samantha Korenek
 Review Date: 3/24/2025

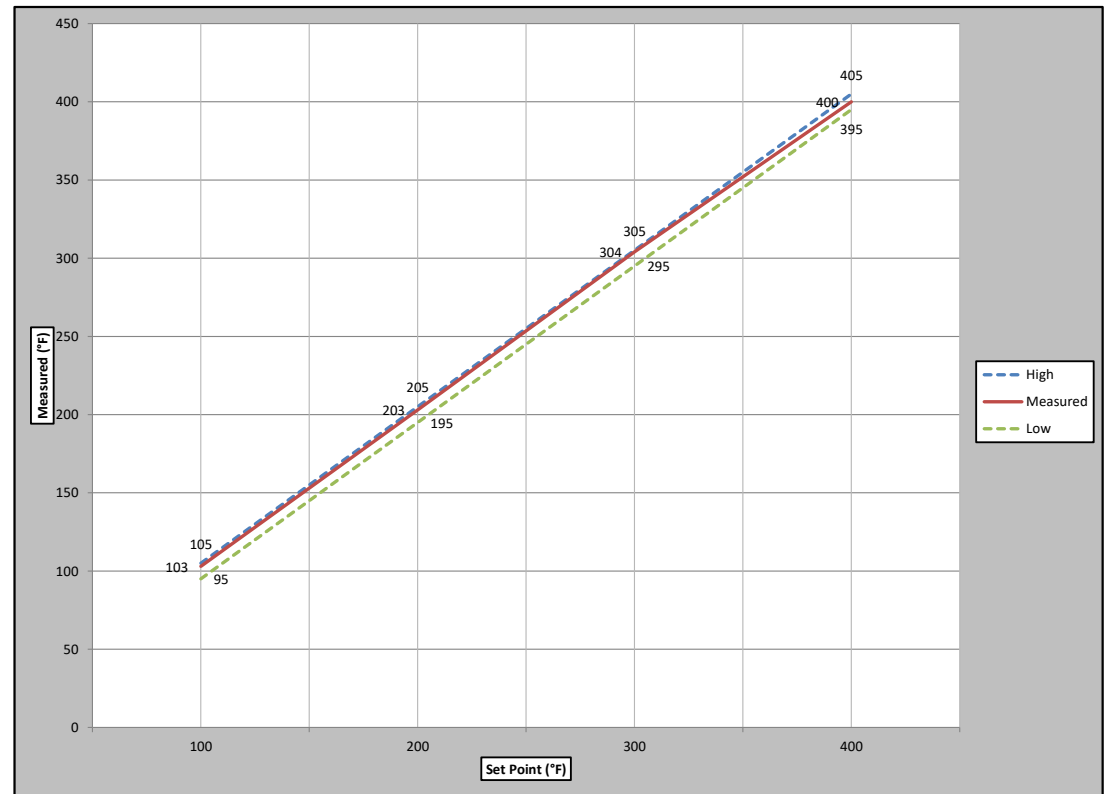

Damage Report
List all damages. Describe how this could have affected measurements.
List all repairs made prior to AS LEFT measurements.
Installed new timer and solid state relay, installed circulation fan and shroud