



Dependable Products From People You Trust

OFI TESTING EQUIPMENT, INC.

11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com


CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

AS FOUND CHART

AS LEFT CHART

| LAB TEMPERATURE | LAB HUMIDITY | PART NUMBER | SERIAL NUMBER | SET POINT | RESULT | ALLOWABLE RANGE | CALIBRATION DATE | DUE DATE | TECHNICIAN |
|-----------------|--------------|-------------|---------------|-----------|----------|-----------------|------------------|-----------|------------|
| 75.00 °F | 57.00 % | 165-00 | 5004250000005 | 930.0 °F | 984.9 °F | 860-1000 °F | 6/16/2025 | 6/16/2026 | SM |

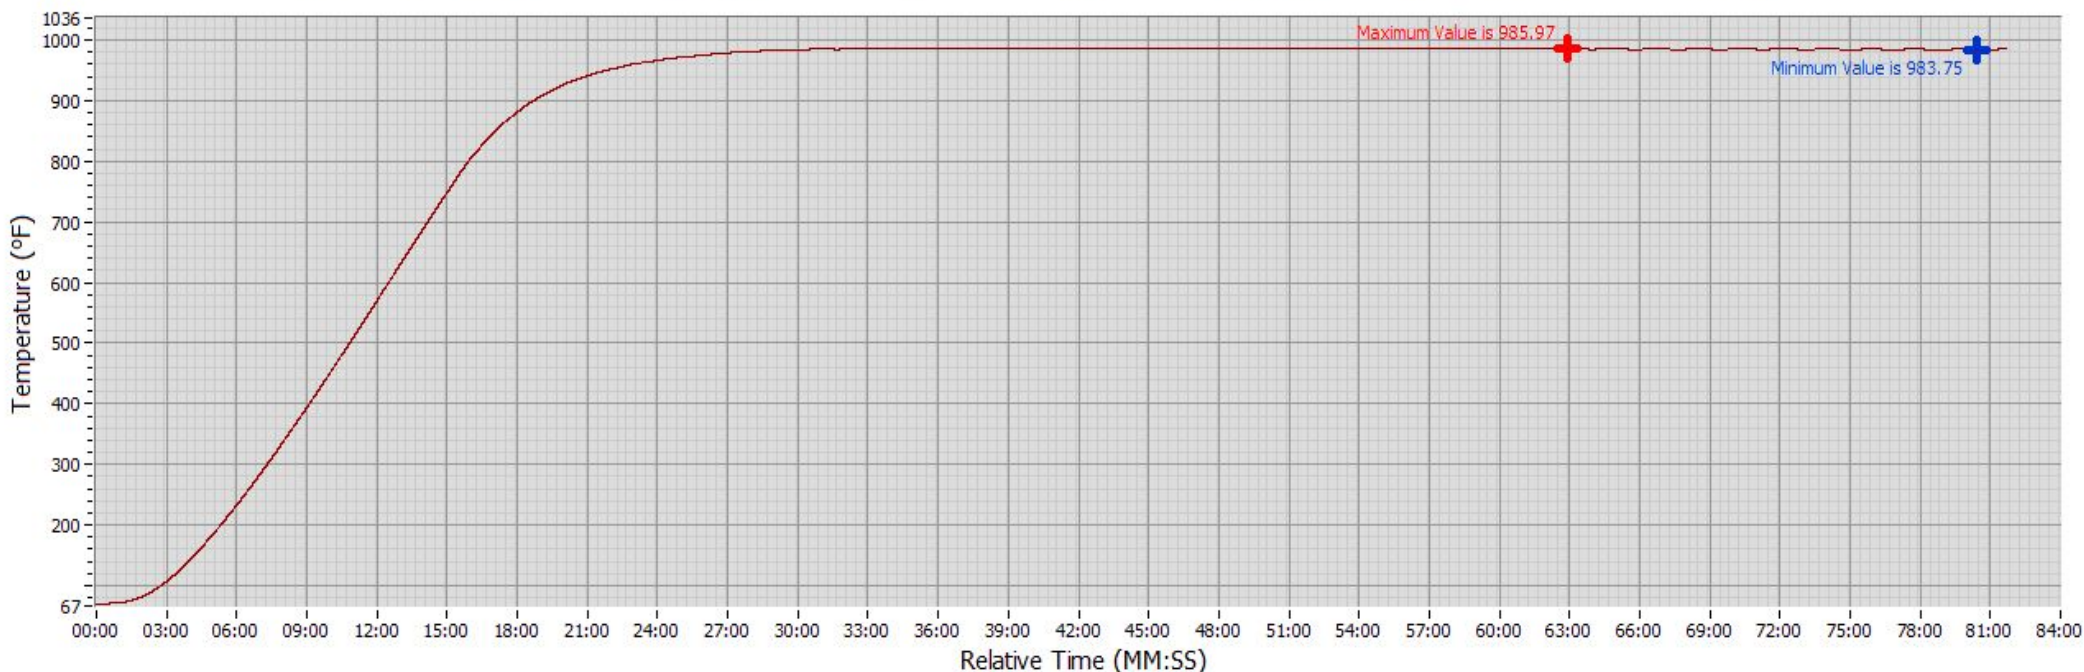

Calibration station has been calibrated using instruments which are traceable to NIST.

| | | |
|---|---|---|
| CAL STATION SERIAL NUMBER: 6B-11 | CAL STATION CALIBRATION DATE: 11/11/2024 | CAL STATION DUE DATE: 11/11/2025 |
| AMBIENT MONITOR MODEL: RH300 | AMBIENT MONITOR S/N: Z395285 | AMBIENT MONITOR CAL DATE: 08/20/2024 AMBIENT MONITOR DUE DATE: 08/20/2025 |
| UNCERTAINTY: ± 2.8°C / 5°F | CALIBRATION PROCEDURE USED: Retort Calibration Procedures API RP 13B-1 | |

- Channel 3
- Plot 1
- Plot 2
- Plot 3
- Plot 4

AS FOUND CONDITION:

CALIBRATION RESULT: Accepted