



Dependable Products From People You Trust

OFI TESTING EQUIPMENT, INC.

11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com


CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

AS FOUND CHART

AS LEFT CHART

LAB TEMPERATURE	LAB HUMIDITY	PART NUMBER	SERIAL NUMBER	SET POINT	RESULT	ALLOWABLE RANGE	CALIBRATION DATE	DUE DATE	TECHNICIAN
73.00 °F	51.00 %	170-00-1	5153620000009	375.0 °F	376.1 °F	350-400 °F	6/18/2025	6/18/2026	SM

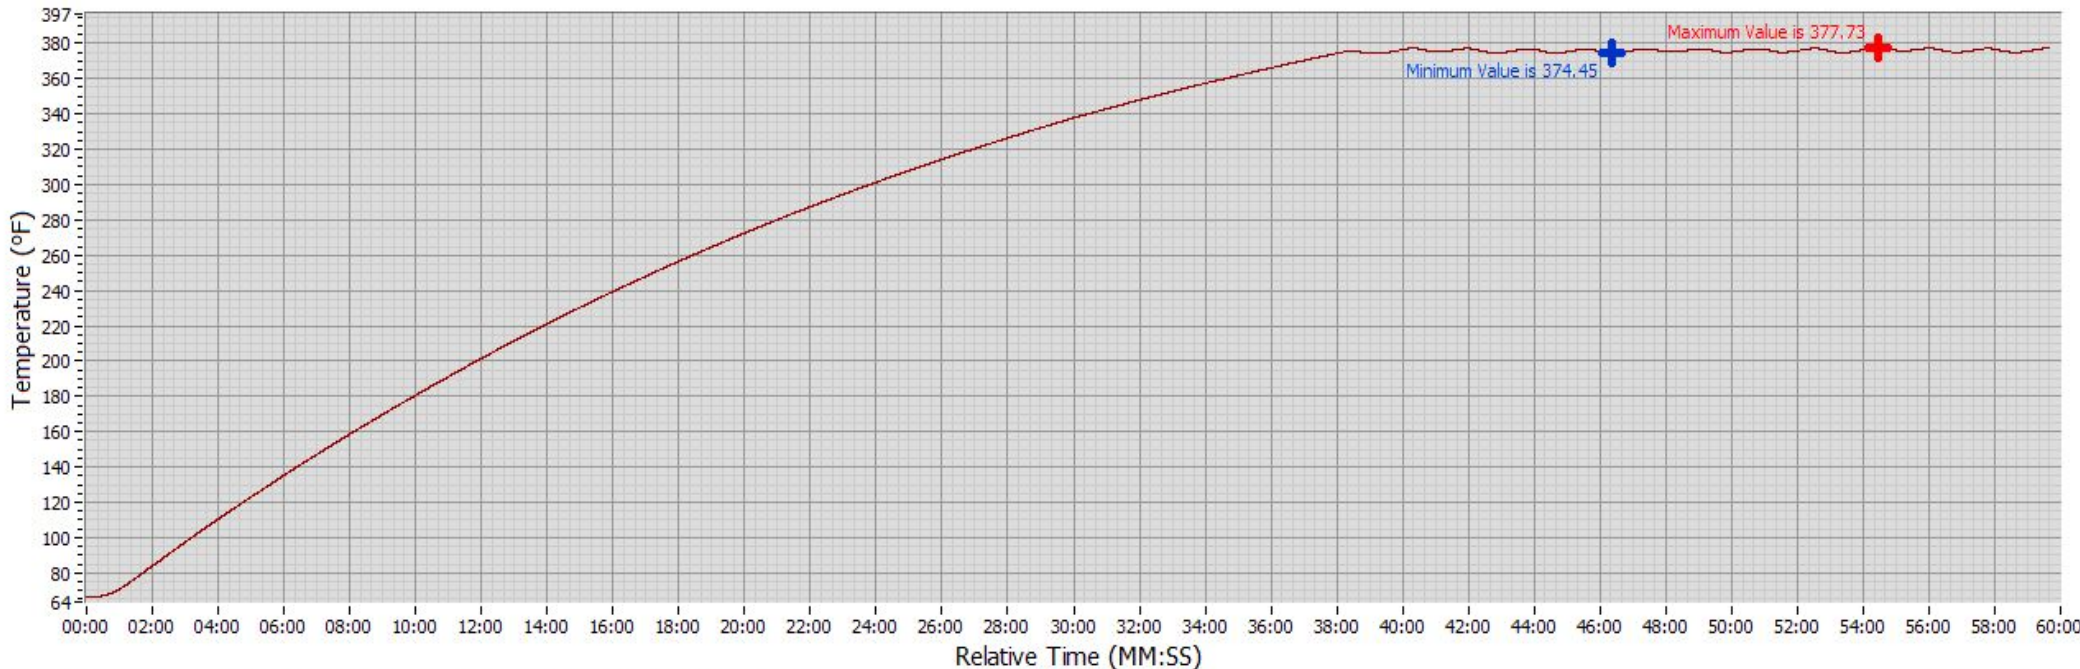

Calibration station has been calibrated using instruments which are traceable to NIST.

CAL STATION SERIAL NUMBER: 6B-11	CAL STATION CALIBRATION DATE: 11/11/2024	CAL STATION DUE DATE: 11/11/2025
AMBIENT MONITOR MODEL: RH300	AMBIENT MONITOR S/N: Z395285	AMBIENT MONITOR CAL DATE: 08/20/2024 AMBIENT MONITOR DUE DATE: 08/20/2025
UNCERTAINTY: ± 2.8°C / 5°F	CALIBRATION PROCEDURE USED: 175 ml Heat Jacket Calibration Procedures API RP 13B-1	

- Channel 1
- Plot 1
- Plot 2
- Plot 3
- Plot 4

AS FOUND CONDITION:

CALIBRATION RESULT: Accepted