



Dependable Products From People You Trust

# OFI TESTING EQUIPMENT, INC.

11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com


## CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

AS FOUND CHART

AS LEFT CHART

LAB TEMPERATURE	LAB HUMIDITY	PART NUMBER	SERIAL NUMBER	SET POINT	RESULT	ALLOWABLE RANGE	CALIBRATION DATE	DUE DATE	TECHNICIAN
73.00 °F	51.00 %	170-00-1	11-2564	375.0 °F	374.5 °F	350-400 °F	6/18/2025	6/18/2026	SM

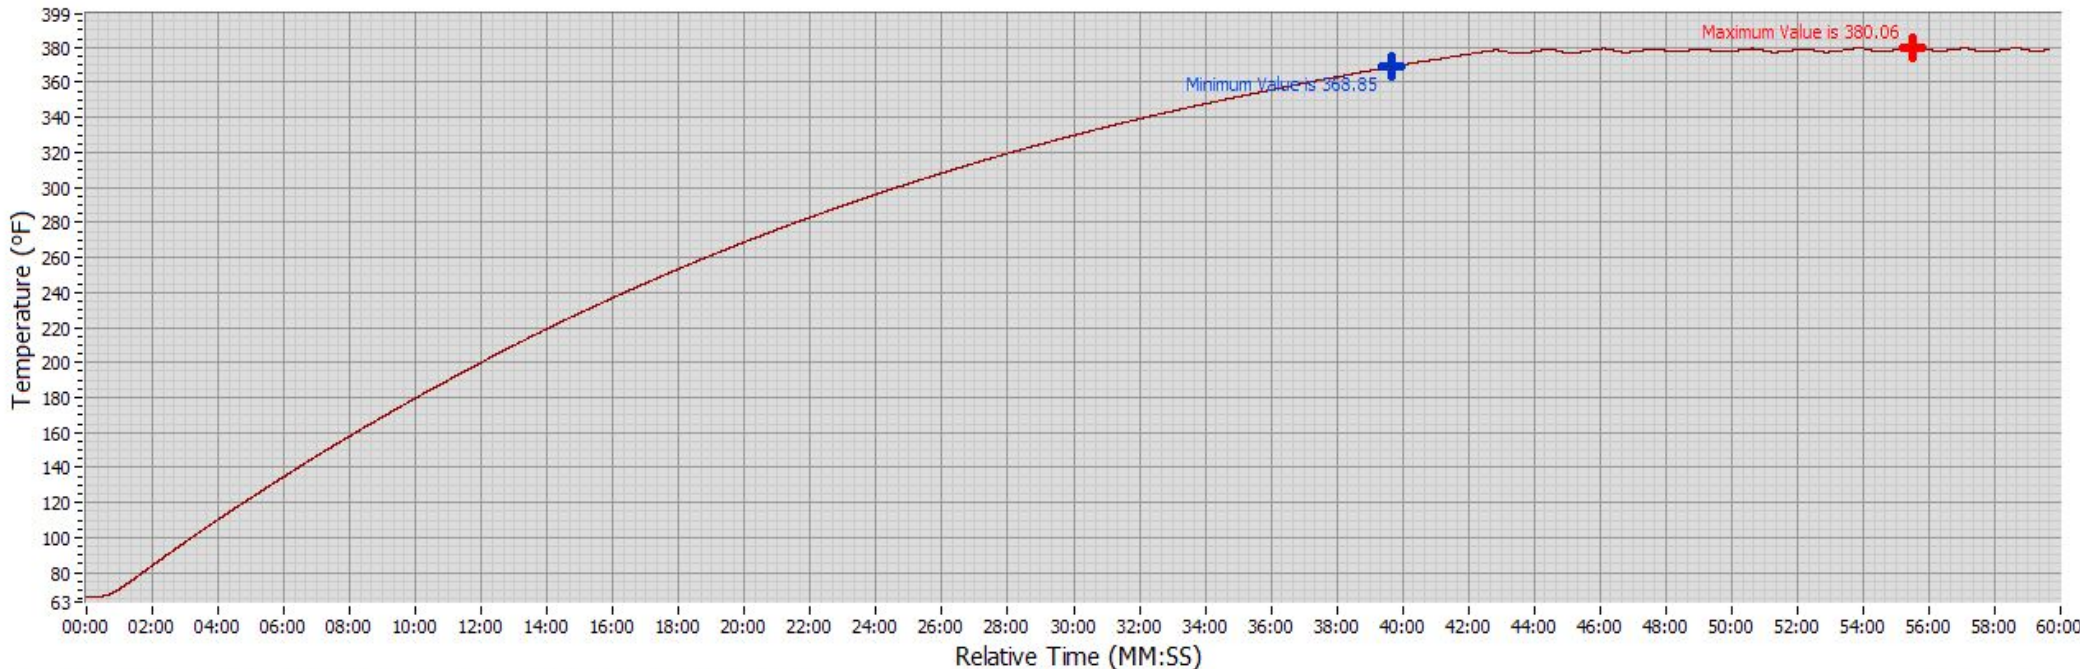

Calibration station has been calibrated using instruments which are traceable to NIST.

**CAL STATION SERIAL NUMBER:** 6B-11      **CAL STATION CALIBRATION DATE:** 11/11/2024      **CAL STATION DUE DATE:** 11/11/2025

**AMBIENT MONITOR MODEL:** RH300      **AMBIENT MONITOR S/N:** Z395285      **AMBIENT MONITOR CAL DATE:** 08/20/2024      **AMBIENT MONITOR DUE DATE:** 08/20/2025

**UNCERTAINTY:** ± 2.8°C / 5°F      **CALIBRATION PROCEDURE USED:** 175 ml Heat Jacket Calibration Procedures API RP 13B-1

- Channel 3
- Plot 1
- Plot 2
- Plot 3
- Plot 4

AS FOUND CONDITION:

CALIBRATION RESULT: Accepted