



# Roller Oven Calibration Report

Order Number:	22723
Serial # / Local I.D. #:	CAL-268
Calibration Date:	6/26/2025
Recommended Due Date:	6/26/2026
Certificate Number:	CAL-26845834
Manufacturer:	OFI Testing Equipment
Part Number:	173-00-C


Condition Found:	In Calibration
Condition Left:	In Calibration
Repairs Required:	Yes
Static Oven:	No
( F ) or ( C ):	(°F)
Max Temp:	400
As Found Required:	No

OFI Testing Equipment, Inc. - 11302 Steeplecrest Dr - Houston, Texas - 77065 - Phone: 832.320.7300 - Web: www.ofite.com

Calibration Equipment						
Thermometer	705	EA10	Z414473	C-38876	7/24/2024	7/24/2025
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Tachometer	312	461920	12050313	C-40454	8/20/2024	8/20/2025
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Ambient Monitor	345	RH300	Z395285	C-40456	8/20/2024	8/20/2025
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Ambient Conditions	Lab / Room Temperature		74	(°F)	Lab / Room Humidity	59.0 %

AS LEFT MEASUREMENTS		(°F)	Max Oven Temp	400	
Set point	Process Temperature	Accepted Deviation	Actual Deviation	Pass/Fail	
100.0	103.4	5.0	3.4	Pass	
	Pass				
200.0	199.8	5.0	-0.2	Pass	
	Pass				
300.0	304.9	5.0	4.9	Pass	
	Pass				
400.0	405.0	5.0	5.0	Pass	
	Pass				
25 RPM	23.4	2	-1.6	Pass	
	Pass				
					Pass

Calibration Technician: Shawn Maglitto  
 Date: 6/26/2025  
 Reviewed By: Samantha Korenek  
 Review Date: 6/30/2025

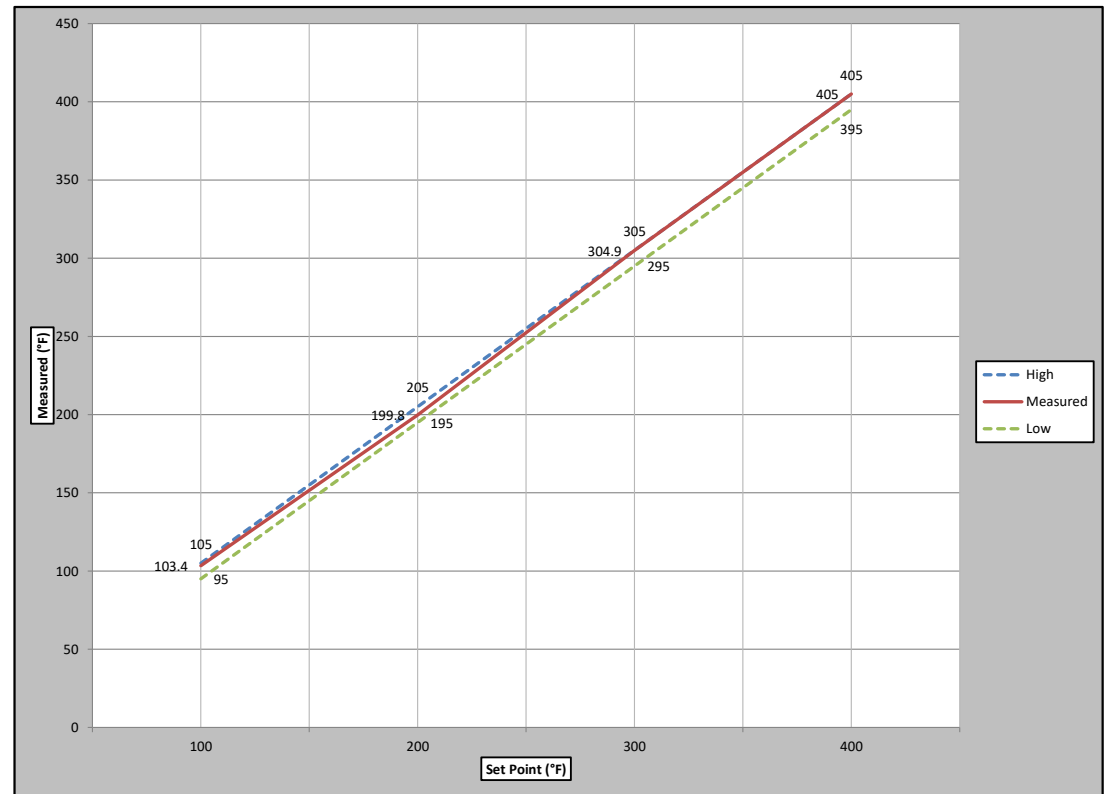

Damage Report
List all damages. Describe how this could have affected measurements.
List all repairs made prior to AS LEFT measurements.