



Dependable Products From People You Trust

# OFI TESTING EQUIPMENT, INC.

11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com


## CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

AS FOUND CHART

AS LEFT CHART

LAB TEMPERATURE	LAB HUMIDITY	PART NUMBER	SERIAL NUMBER	SET POINT	RESULT	ALLOWABLE RANGE	CALIBRATION DATE	DUE DATE	TECHNICIAN
73.00 °F	51.00 %	171-01-1	5392340000004	450.0 °F	450.9 °F	425-475 °F	7/3/2025	7/3/2026	SM

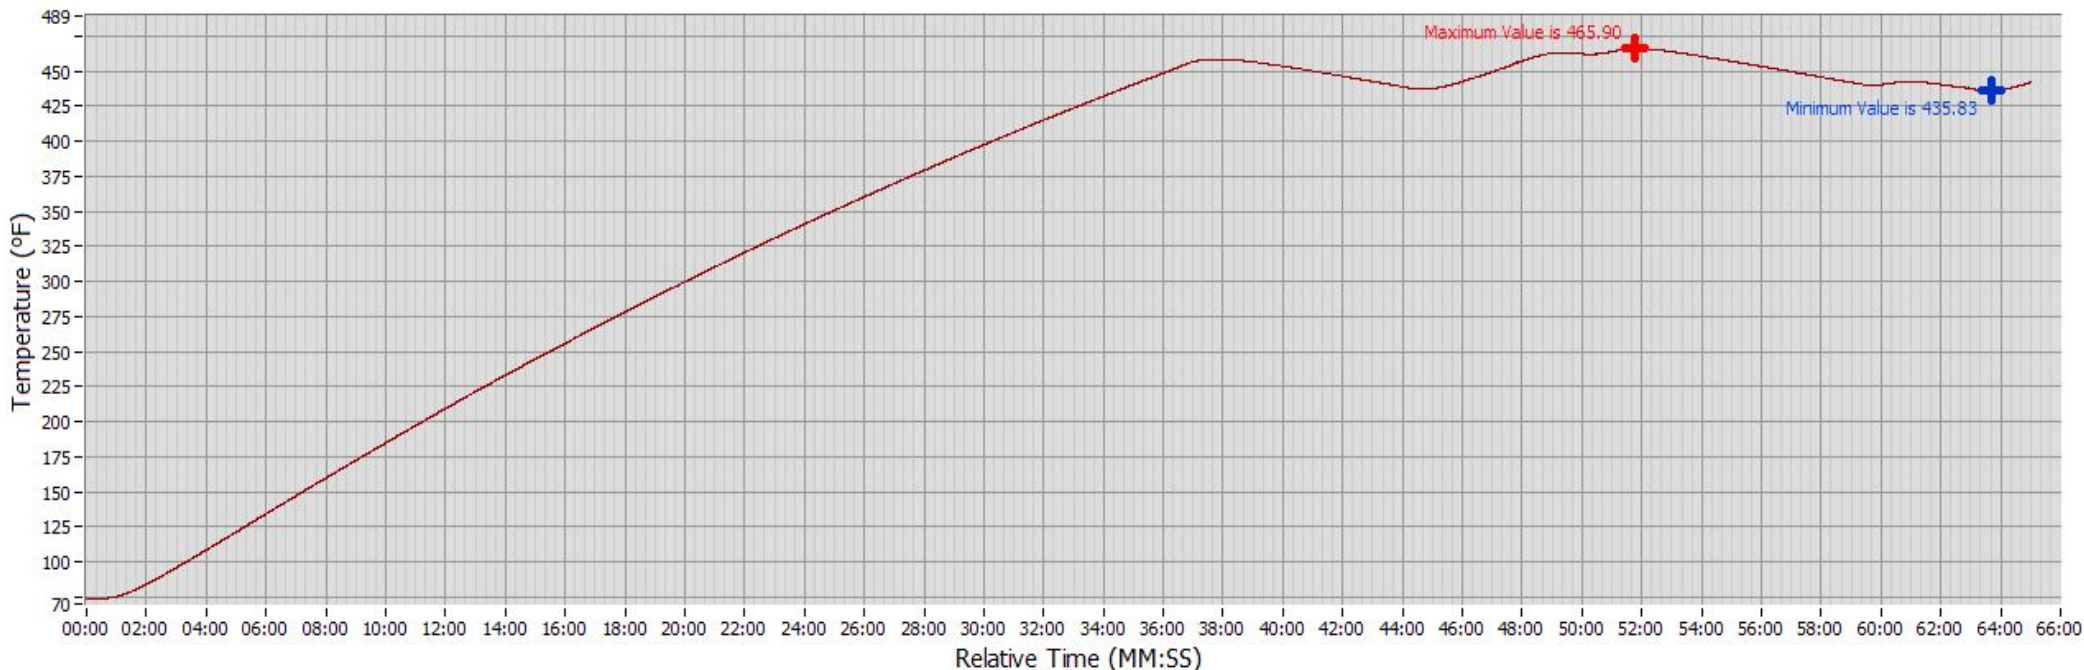

Calibration station has been calibrated using instruments which are traceable to NIST.

<b>CAL STATION SERIAL NUMBER:</b> 6B-11	<b>CAL STATION CALIBRATION DATE:</b> 11/11/2024	<b>CAL STATION DUE DATE:</b> 11/11/2025
<b>AMBIENT MONITOR MODEL:</b> RH300	<b>AMBIENT MONITOR S/N:</b> Z395285	<b>AMBIENT MONITOR CAL DATE:</b> 08/20/2024 <b>AMBIENT MONITOR DUE DATE:</b> 08/20/2025
<b>UNCERTAINTY:</b> ± 2.8°C / 5°F	<b>CALIBRATION PROCEDURE USED:</b> 500 ml Heat Jacket Calibration Procedures API RP 13B-2	

- Channel 4
- Plot 1
- Plot 2
- Plot 3
- Plot 4

AS FOUND CONDITION:

CALIBRATION RESULT: Accepted