



Dependable Products From People You Trust

OFI TESTING EQUIPMENT, INC.


11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com

CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

- AS FOUND CHART
- AS LEFT CHART

LAB TEMPERATURE	LAB HUMIDITY	PART NUMBER	SERIAL NUMBER	SET POINT	RESULT	ALLOWABLE RANGE	CALIBRATION DATE	DUE DATE	TECHNICIAN
74.00 °F	43.00 %	171-01-1	539234000005	450.0 °F	453.7 °F	425-475 °F	7/2/2025	7/2/2026	SM

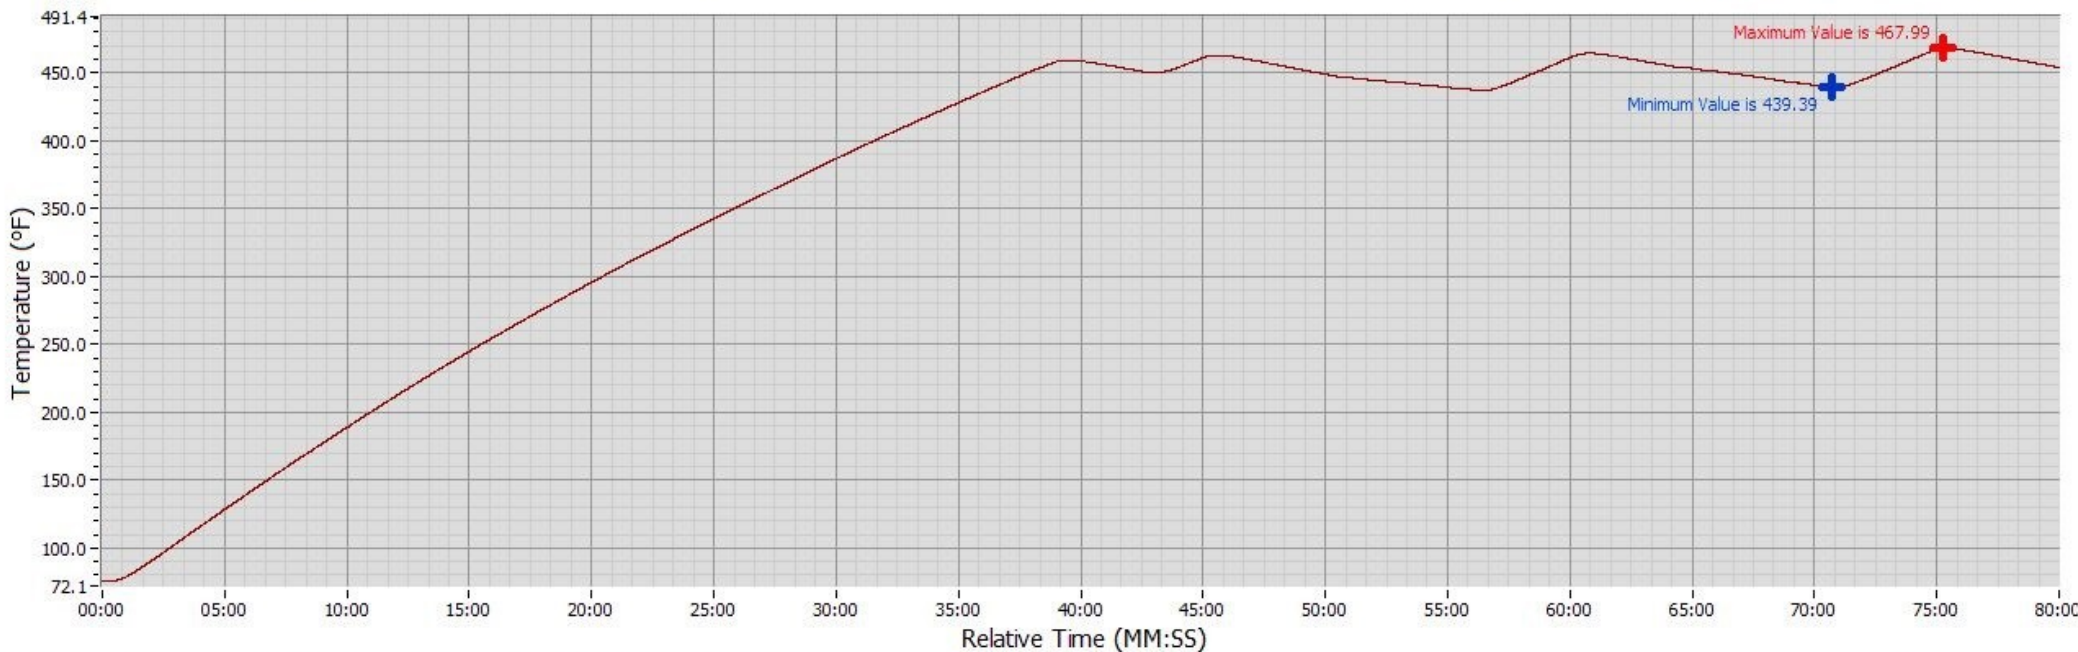

Calibration station has been calibrated using instruments which are traceable to NIST.

Channel 5

CAL STATION SERIAL NUMBER: 6B-11
CAL STATION CALIBRATION DATE: 11/11/2024
CAL STATION DUE DATE: 11/11/2025
AMBIENT MONITOR MODEL: RH300
AMBIENT MONITOR S/N: Z395285
AMBIENT MONITOR CAL DATE: 08/20/2024
AMBIENT MONITOR DUE DATE: 08/20/2025
UNCERTAINTY: ± 2.8°C / 5°F
CALIBRATION PROCEDURE USED 500 ml Heat Jacket Calibration Procedures API RP 13B-2

AS FOUND CONDITION:

CALIBRATION RESULT: Accepted