




| | |
|------------------------|--------------------|
| Order Number: | NEW |
| Serial# / Local I.D. # | 5382900000001 |
| Calibration Date: | 8/19/2025 |
| Recommended Due Date: | 8/19/2026 |
| Certificate Number: | 538290000000145888 |
| Condition Found: | NEW |
| Condition Left: | In Calibration |
| Cell Serial Number: | 0047559-06 |

11302 Steeplecrest Dr - Houston, Texas - 77065 - Phone: 832.320.7300 - E-Mail: www.ofite.com

120-35 / 25,000 - 400°F / Automated HTHP Consistometer

| CONSISTENCY READING OF POTENTIOMETER | | |
|--------------------------------------|--------------|-------------|
| MASS (g) | OUTPUT (VDC) | CONSISTENCY |
| 0 | 0.0 | 0.0 |
| 50 | 1.0 | 11.2 |
| 100 | 2.0 | 21.7 |
| 150 | 3.3 | 34.6 |
| 200 | 4.4 | 45.4 |
| 250 | 5.9 | 60.9 |
| 300 | 7.2 | 73.6 |
| 350 | 8.6 | 87.8 |
| 400 | 9.9 | 100.8 |

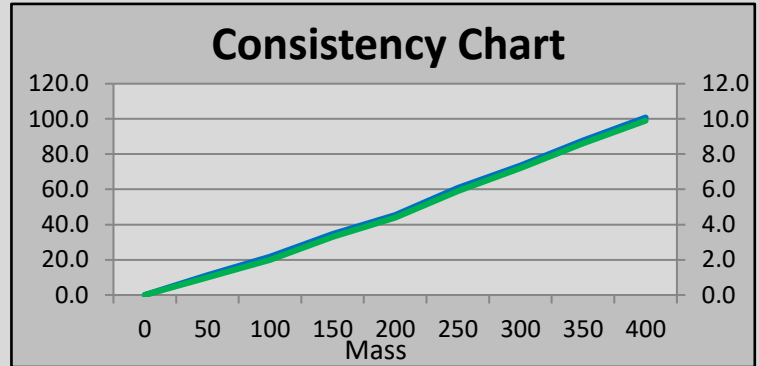

Potentiometer S/N: 5382900000001

MOTOR SPEED ACCURACY CHECK

| Target Speed | Measured Tachometer Speed | Allowed Deviation | Actual Deviation | Pass / Fail |
|-------------------|---------------------------|--------------------------------|------------------|-------------|
| 150 RPM | 149.8 | ± 15 RPM | 0 RPM | Pass |
| | Pass | | | |
| Tachometer I.D. # | 678 | Calibration Certificate Number | C-52609 | |
| Model Number | R7050 | Calibration Date | 7/23/2025 | |
| Serial Number | 220326760 | Calibration Due Date | 7/23/2026 | |

TEMPERATURE CALIBRATION

| SAMPLE | THERMOCOUPLE | 100 | 200 | 400 | 600 | ALLOWED DEVIATION | °F or °C | °F | PASS / FAIL |
|-------------------|--------------|--------------|--------|--------------------------------|----------------------|-------------------|------------------|------------|-------------|
| | | | | | | | ACTUAL DEVIATION | | |
| CONTROLLER/AMULET | | 98.30 | 200.30 | 400.00 | NA | 2.00 | 1.70 | | Pass |
| | | Pass | Pass | Pass | Pass | | | | |
| SOFTWARE) | | 98.30 | 200.30 | 400.00 | NA | 2.00 | 1.70 | | Pass |
| | | Pass | Pass | Pass | Pass | | | | |
| Dry Block I.D. # | | 674 | | Calibration Certificate Number | | | C-43025 | | |
| Model Number | | ETC-400A 11 | | | Calibration Date | | | 10/23/2024 | |
| Serial Number | | 692360-02363 | | | Calibration Due Date | | | 10/23/2025 | |

PRESSURE TRANSDUCER / GAUGE

| CALIBRATION PRESSURES (PSI) | CALIBRATED GAUGE (PSI) | AMULET UNIT | | | SOFTWARE (PSI) | MAWP of Machine (PSI) | 25000 | PASS / FAIL |
|-----------------------------|------------------------|---------------------|--------------------------------|------------------------|----------------------|-----------------------|-------|-------------|
| | | MACHINE GAUGE (PSI) | MACHINE AMULET (PSI) | ALLOWED DEVIATION (1%) | | | | |
| 25% MAWP | 6,250 | 6,250.0 | 6,250.0 | 6,273.0 | 6,273.0 | 250.0 | 23 | Pass |
| | | Pass | Pass | Pass | Pass | | | |
| 50% MAWP | 12,500 | 12,500.0 | 12,550.0 | 12,522.0 | 12,522.0 | 250.0 | 50 | Pass |
| | | Pass | Pass | Pass | Pass | | | |
| 75% MAWP | 18,750 | 18,750.0 | 18,750.0 | 18,739.0 | 18,739.0 | 250.0 | 11 | Pass |
| | | Pass | Pass | Pass | Pass | | | |
| Calibrated Gauge I.D. # | | 157 | Calibration Certificate Number | | | C-52337 | | |
| Model Number | | JHW60KGZ | | | Calibration Date | | | 7/7/2025 |
| Serial Number | | 1391934 | | | Calibration Due Date | | | 7/7/2026 |

This report meets or exceeds the requirements outlined in API RP 10B-2 Recommended Practice for Testing Well Cements for calibration of laboratory devices, using certified master test equipment that is traceable to NIST which is a signatory to the Mutual Recognition Arrangement (MRA) with the International Laboratory Accreditation Cooperation (ILAC).

Ebram Azer
CALIBRATED BY

8/19/2025
DATE

Samantha Korenek
REVIEWED BY

8/19/2025
DATE