



## Roller Oven Calibration Report


|                          |                       |
|--------------------------|-----------------------|
| Order Number:            | NEW                   |
| Serial # / Local I.D. #: | 5017610000001         |
| Calibration Date:        | 12/12/2025            |
| Recommended Due Date:    | 12/12/2026            |
| Certificate Number:      | 501761000000146003    |
| Manufacturer:            | OFI Testing Equipment |
| Part Number:             | 173-00-RC             |

|                    |                |
|--------------------|----------------|
| Condition Found:   | NEW            |
| Condition Left:    | In Calibration |
| Repairs Required:  | No             |
| Static Oven:       | No             |
| (F) or (C):        | (°F)           |
| Max Temp:          | 500            |
| As Found Required: | No             |

OFI Testing Equipment, Inc. - 11302 Steeplecrest Dr - Houston, Texas - 77065 - Phone: 832.320.7300 - Web: www.ofite.com

| Calibration Equipment |                        |              |               |                    |                     |                      |
|-----------------------|------------------------|--------------|---------------|--------------------|---------------------|----------------------|
| Thermometer           | 705                    | EA10         | Z414473       | C-52618            | 7/23/2025           | 7/23/2026            |
|                       | I.D. Number            | Model Number | Serial Number | Certificate Number | Calibration Date    | Calibration Due Date |
| Tachometer            | 173                    | 461920       | 131105905     | C-46744            | 2/6/2025            | 2/6/2026             |
|                       | I.D. Number            | Model Number | Serial Number | Certificate Number | Calibration Date    | Calibration Due Date |
| Ambient Monitor       | 728                    | RH300        | Z430119       | 305923             | 4/1/2025            | 4/1/2026             |
|                       | I.D. Number            | Model Number | Serial Number | Certificate Number | Calibration Date    | Calibration Due Date |
| Ambient Conditions    | Lab / Room Temperature |              | 73.7          | (°F)               | Lab / Room Humidity |                      |
|                       |                        |              |               |                    | 53.9 %              |                      |

| AS LEFT MEASUREMENTS |                     | (°F)               | Max Oven Temp    | 500       |      |
|----------------------|---------------------|--------------------|------------------|-----------|------|
| Set point            | Process Temperature | Accepted Deviation | Actual Deviation | Pass/Fail |      |
| 100.0                | 99.2                | 5.0                | -0.8             | Pass      |      |
|                      | Pass                |                    |                  |           |      |
| 200.0                | 200.5               | 5.0                | 0.5              | Pass      |      |
|                      | Pass                |                    |                  |           |      |
| 300.0                | 300.4               | 5.0                | 0.4              | Pass      |      |
|                      | Pass                |                    |                  |           |      |
| 400.0                | 400.8               | 5.0                | 0.8              | Pass      |      |
|                      | Pass                |                    |                  |           |      |
| 500.0                | 501.2               | 5.0                | 1.2              | Pass      |      |
|                      | Pass                |                    |                  |           |      |
| 25 RPM               | 25.3                | 2                  | 0.3              | Pass      |      |
|                      | Pass                |                    |                  |           |      |
|                      |                     |                    |                  |           | Pass |

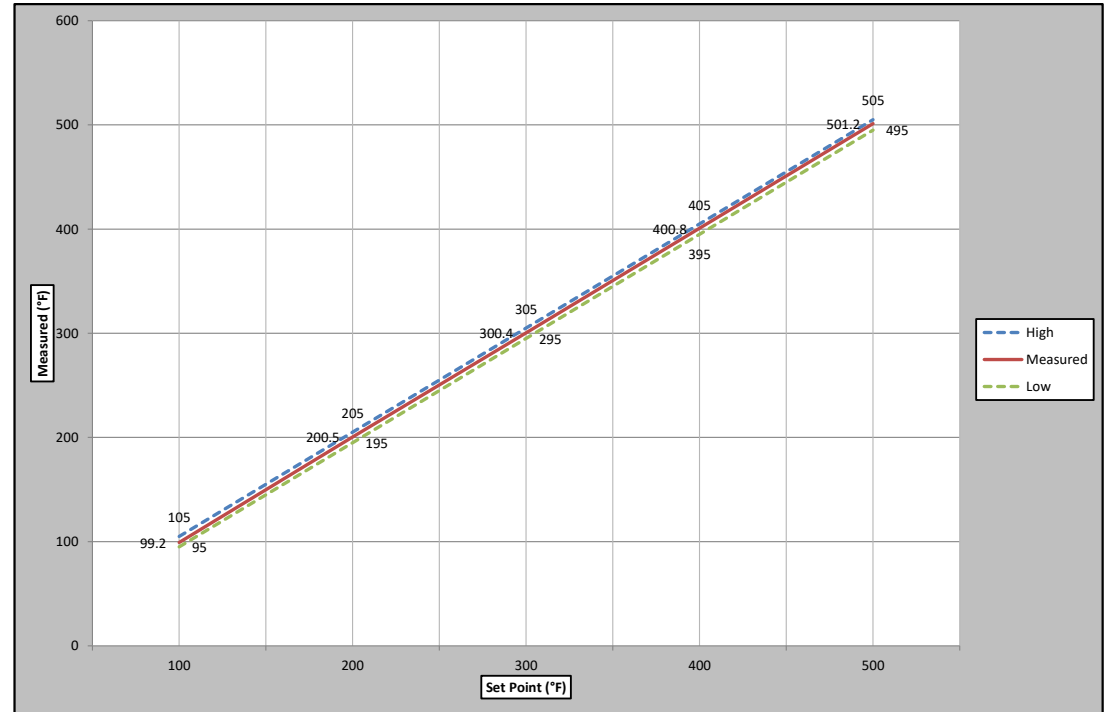

Calibration Technician: Benjamin McMullin

Technician Signature: *Benjamin McMullin*

Date: 12/12/2025

Reviewed By: Samantha Korenek

Reviewer Signature: *Samantha Korenek*

Review Date: 12/15/2025