



Dependable Products From People You Trust

# OFI TESTING EQUIPMENT, INC.

11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com


## CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

AS FOUND CHART

AS LEFT CHART

LAB TEMPERATURE	LAB HUMIDITY	PART NUMBER	SERIAL NUMBER	SET POINT	RESULT	ALLOWABLE RANGE	CALIBRATION DATE	DUE DATE	TECHNICIAN
70.00 °F	23.00 %	165-14-1	5402370000004	930.0 °F	971.3 °F	860-1000 °F	12/30/2025	12/30/2027	SM

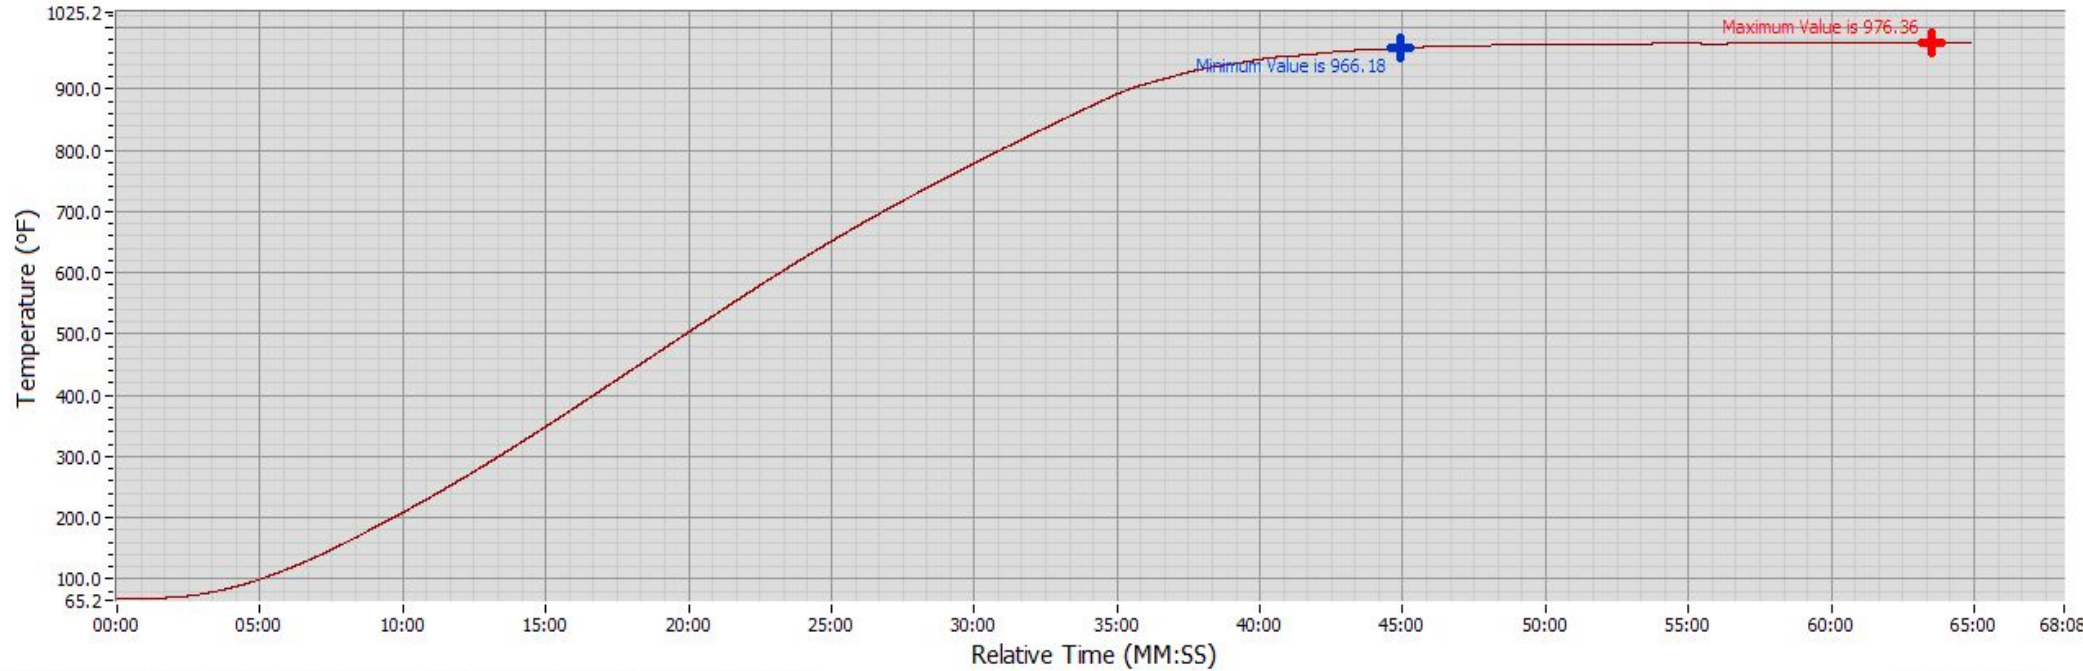

Calibration station has been calibrated using instruments which are traceable to NIST.

Channel 4

**CAL STATION SERIAL NUMBER:** 6B-11    **CAL STATION CALIBRATION DATE:** 11/04/2025    **CAL STATION DUE DATE:** 11/04/2026

**AMBIENT MONITOR MODEL:** RH300    **AMBIENT MONITOR S/N:** Z430119    **AMBIENT MONITOR CAL DATE:** 04/01/2025    **AMBIENT MONITOR DUE DATE:** 04/01/2026

**UNCERTAINTY:** ± 2.8°C / 5°F    **CALIBRATION PROCEDURE USED:** Retort Calibration Procedures API RP 13B-1

**AS FOUND CONDITION:**

**CALIBRATION RESULT:** Accepted