



Roller Oven Calibration Report


Order Number:	NEW
Serial # / Local I.D. #:	540200000001
Calibration Date:	12/31/2025
Recommended Due Date:	12/31/2026
Certificate Number:	540200000000146022
Manufacturer:	OFI Testing Equipment
Part Number:	173-00-1-C

Condition Found:	NEW
Condition Left:	In Calibration
Repairs Required:	No
Static Oven:	No
(F) or (C):	(°F)
Max Temp:	500
As Found Required:	No

OFI Testing Equipment, Inc. - 11302 Steeplecrest Dr - Houston, Texas - 77065 - Phone: 832.320.7300 - Web: www.ofite.com

Calibration Equipment						
Thermometer	173	461920	131105905	C-46744	2/6/2025	2/6/2026
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Tachometer	154	EA10	Z375331	C-52617	7/23/2025	7/23/2026
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Ambient Monitor	728	RH300	Z430119	305923	4/1/2025	4/1/2026
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Ambient Conditions	Lab / Room Temperature		71.2	(°F)	Lab / Room Humidity	
						31.9 %

AS LEFT MEASUREMENTS		(°F)	Max Oven Temp	500	
Set point	Process Temperature	Accepted Deviation	Actual Deviation	Pass/Fail	
100.0	99.0	5.0	-1.0	Pass	
	Pass				
200.0	201.0	5.0	1.0	Pass	
	Pass				
300.0	302.0	5.0	2.0	Pass	
	Pass				
400.0	401.0	5.0	1.0	Pass	
	Pass				
500.0	498.0	5.0	-2.0	Pass	
	Pass				
25 RPM	24.7	2	-0.3	Pass	
	Pass				

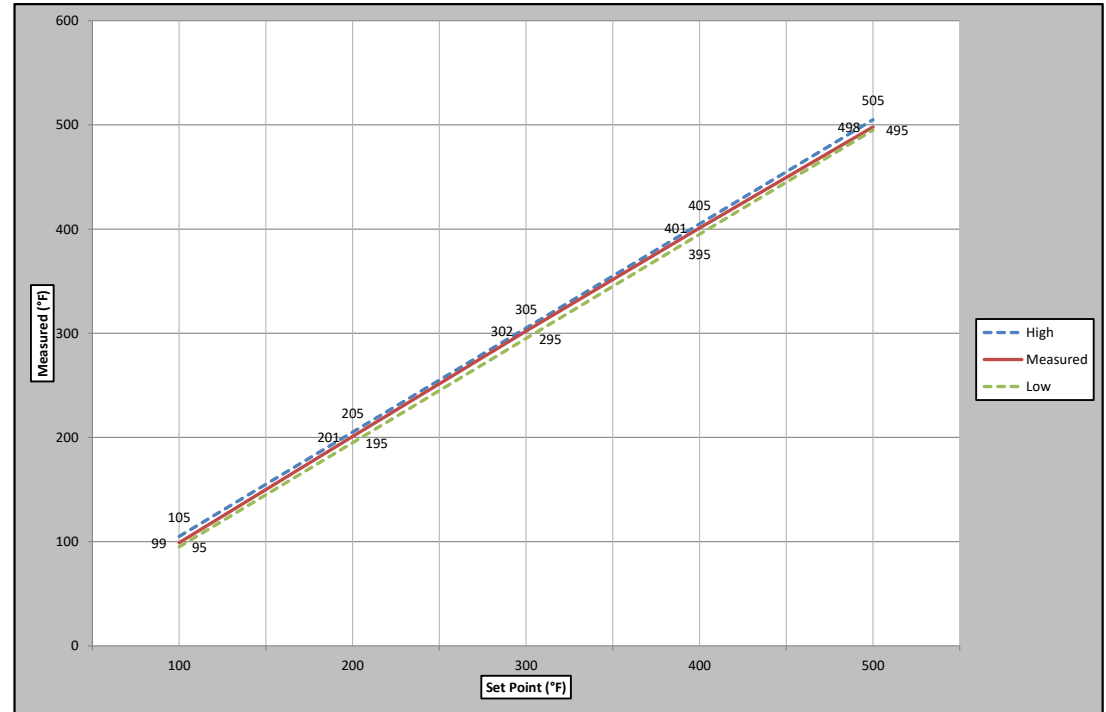

Calibration Technician: Shawn Maglito

Technician Signature: *Shawn Maglito*

Date: 12/31/2025

Reviewed By: Samantha Korenek

Reviewer Signature: *Samantha Korenek*

Review Date: 12/31/2025