



Dependable Products From People You Trust

OFI TESTING EQUIPMENT, INC.


11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com

CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

- AS FOUND CHART
- AS LEFT CHART

LAB TEMPERATURE	LAB HUMIDITY	PART NUMBER	SERIAL NUMBER	SET POINT	RESULT	ALLOWABLE RANGE	CALIBRATION DATE	DUE DATE	TECHNICIAN
73.9 °F	32.3 %	170-00-1	5180500000005	375.0 °F	374.4 °F	350-400 °F	1/7/2026	1/7/2027	SM

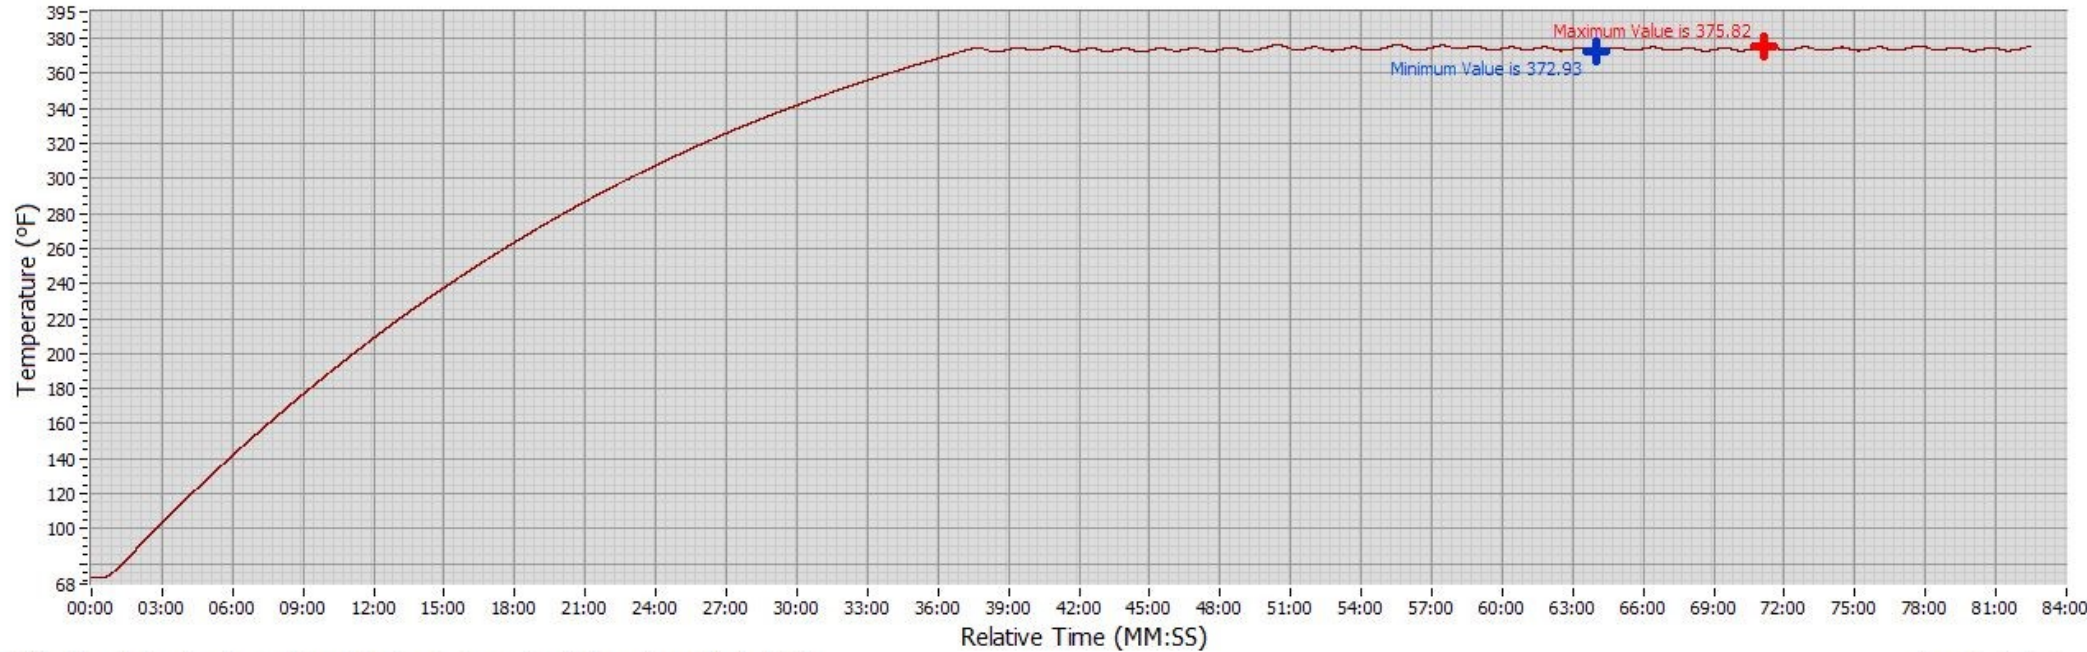

Calibration station has been calibrated using instruments which are traceable to NIST.

CAL STATION SERIAL NUMBER: 6B-11

CAL STATION CALIBRATION DATE: 11/04/2025

CAL STATION DUE DATE: 11/04/2026

AMBIENT MONITOR MODEL: RH300

AMBIENT MONITOR S/N: Z430119

AMBIENT MONITOR CAL DATE: 04/01/2025

AMBIENT MONITOR DUE DATE: 04/01/2026

UNCERTAINTY: ± 2.8°C / 5°F

CALIBRATION PROCEDURE USED: 175 ml Heat Jacket Calibration Procedures API RP 13B-1

AS FOUND CONDITION:

CALIBRATION RESULT: Accepted

- Channel 2
- Plot 1
- Plot 2
- Plot 3
- Plot 4