



Roller Oven Calibration Report


Order Number:	540477
Serial # / Local I.D. #:	5404770000001
Calibration Date:	1/29/2026
Recommended Due Date:	1/29/2027
Certificate Number:	540477000000146051
Manufacturer:	OFI Testing Equipment
Part Number:	172-00-99

Condition Found:	In Calibration
Condition Left:	In Calibration
Repairs Required:	Yes
Static Oven:	No
(F) or (C):	(°F)
Max Temp:	500
As Found Required:	No

OFI Testing Equipment, Inc. - 11302 Steeplecrest Dr - Houston, Texas - 77065 - Phone: 832.320.7300 - Web: www.ofite.com

Calibration Equipment						
Thermometer	154	EA10	Z375331	C-52617	7/23/2025	7/23/2026
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Tachometer	706	R7050	220502483	C-54329	9/5/2025	9/5/2026
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Ambient Monitor	728	RH300	Z430119	305923	4/1/2025	4/1/2026
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Ambient Conditions	Lab / Room Temperature		70.3	(°F)	Lab / Room Humidity	
						28.2 %

AS LEFT MEASUREMENTS		(°F)	Max Oven Temp	500	
Set point	Process Temperature	Accepted Deviation	Actual Deviation	Pass/Fail	
100.0	101.0	5.0	1.0	Pass	
	Pass				
200.0	203.0	5.0	3.0	Pass	
	Pass				
300.0	304.0	5.0	4.0	Pass	
	Pass				
400.0	404.0	5.0	4.0	Pass	
	Pass				
500.0	503.0	5.0	3.0	Pass	
	Pass				
25 RPM	24.6	2	-0.4	Pass	
	Pass				
					Pass

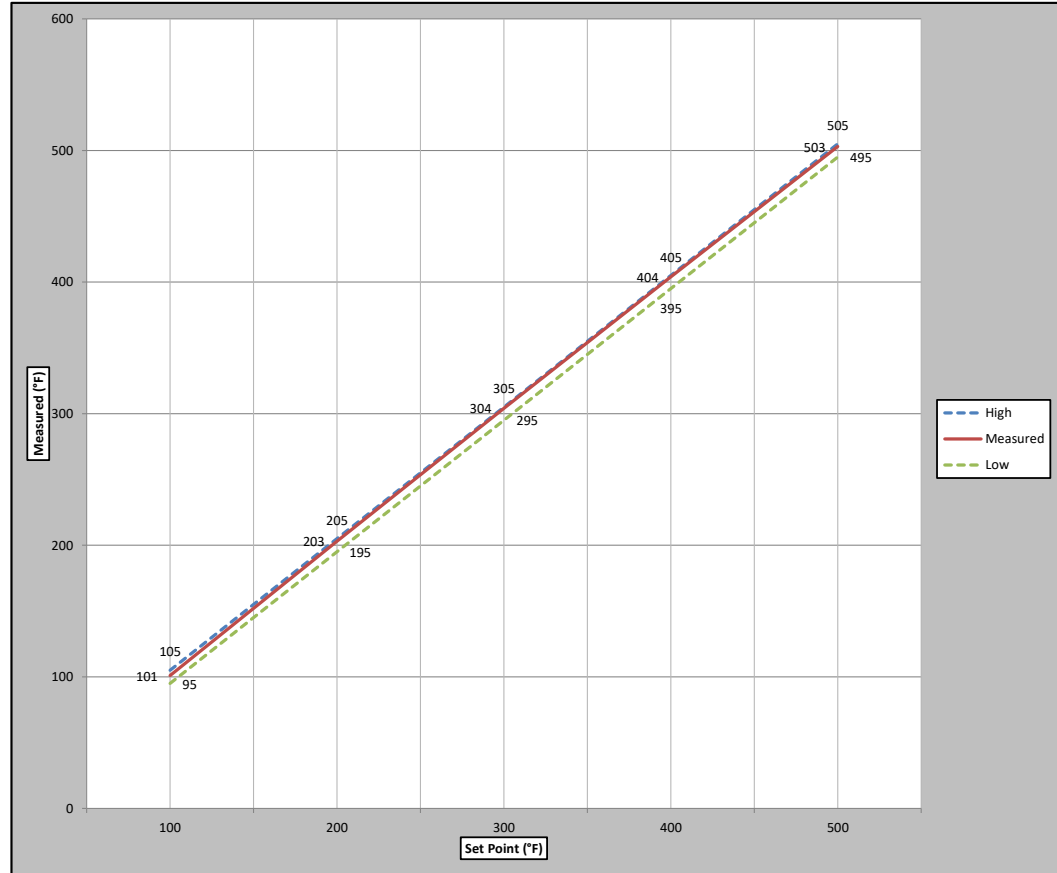

Calibration Technician: Shawn Maglito
 Technician Signature: *Shawn Maglito*
 Date: 1/29/2026
 Reviewed By: Samantha Korenek
 Reviewer Signature: *Samantha Korenek*
 Review Date: 1/29/2026

Damage Report	
List all damages. Describe how this could have affected measurements.	
List all repairs made prior to AS LEFT measurements.	