



Roller Oven Calibration Report


Order Number:	540477
Serial # / Local I.D. #:	5404770000002
Calibration Date:	1/29/2026
Recommended Due Date:	1/29/2027
Certificate Number:	540477000000246051
Manufacturer:	OFI Testing Equipment
Part Number:	172-00-99

Condition Found:	In Calibration
Condition Left:	In Calibration
Repairs Required:	Yes
Static Oven:	No
(F) or (C):	(°F)
Max Temp:	500
As Found Required:	No

OFI Testing Equipment, Inc. - 11302 Steeplecrest Dr - Houston, Texas - 77065 - Phone: 832.320.7300 - Web: www.ofite.com

Calibration Equipment						
Thermometer	154	EA10	Z375331	C-52617	7/23/2025	7/23/2026
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Tachometer	706	R7050	220502483	C-54329	9/5/2025	9/5/2026
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Ambient Monitor	728	RH300	Z430119	305923	4/1/2025	4/1/2026
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Ambient Conditions	Lab / Room Temperature		70.3	(°F)	Lab / Room Humidity	
					28.2 %	

AS LEFT MEASUREMENTS		(°F)	Max Oven Temp	500	
Set point	Process Temperature	Accepted Deviation	Actual Deviation	Pass/Fail	
100.0	98.0	5.0	-2.0	Pass	
	Pass				
200.0	202.0	5.0	2.0	Pass	
	Pass				
300.0	303.0	5.0	3.0	Pass	
	Pass				
400.0	400.0	5.0	0.0	Pass	
	Pass				
500.0	499.0	5.0	-1.0	Pass	
	Pass				
25 RPM	25.5	2	0.5	Pass	
	Pass				
					Pass

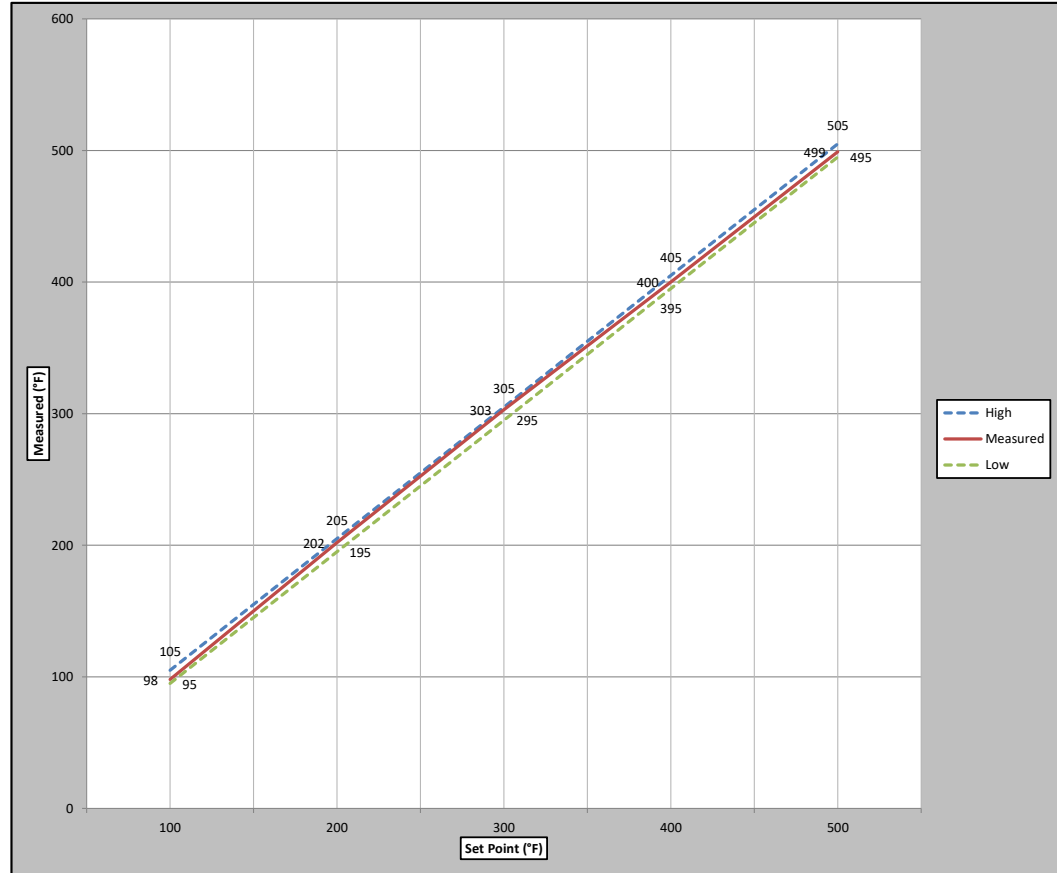

Calibration Technician: Shawn Maglito

Technician Signature: *Shawn Maglito*

Date: 1/29/2026

Reviewed By: Samantha Korenek

Reviewer Signature: *Samantha Korenek*

Review Date: 1/29/2026

Damage Report	
List all damages. Describe how this could have affected measurements.	
List all repairs made prior to AS LEFT measurements.	