



Dependable Products From People You Trust

# OFI TESTING EQUIPMENT, INC.


11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com

## CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

- AS FOUND CHART
- AS LEFT CHART

LAB TEMPERATURE	LAB HUMIDITY	PART NUMBER	SERIAL NUMBER	SET POINT	RESULT	ALLOWABLE RANGE	CALIBRATION DATE	DUE DATE	TECHNICIAN
69.20 °F	53.10 %	165-14-3	5404340000004	930.0 °F	915.1 °F	860-1000 °F	2/11/2026	2/11/2027	SM

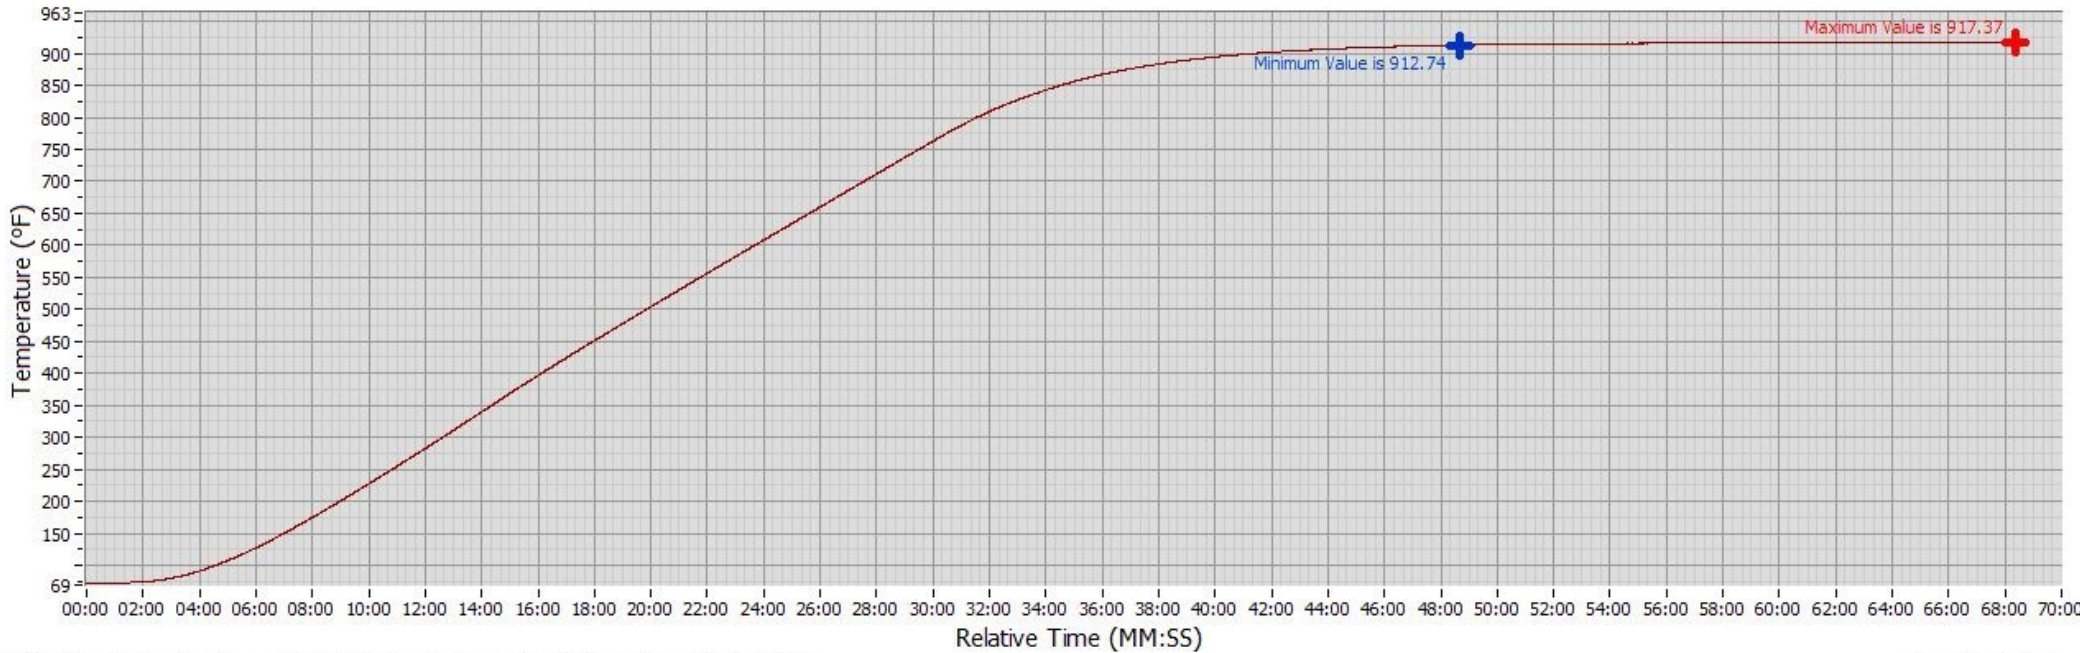

Calibration station has been calibrated using instruments which are traceable to NIST.

**CAL STATION SERIAL NUMBER:** 6B-11      **CAL STATION CALIBRATION DATE:** 11/04/2025      **CAL STATION DUE DATE:** 11/04/2026

**AMBIENT MONITOR MODEL:** RH300      **AMBIENT MONITOR S/N:** Z430119      **AMBIENT MONITOR CAL DATE:** 04/01/2025      **AMBIENT MONITOR DUE DATE:** 04/01/2026

**UNCERTAINTY:** ± 2.8°C / 5°F      **CALIBRATION PROCEDURE USED:** Retort Calibration Procedures API RP 13B-1

- Channel 4
- Plot 1
- Plot 2
- Plot 3
- Plot 4

**AS FOUND CONDITION:**

**CALIBRATION RESULT:** Accepted