



Dependable Products From People You Trust

# OFI TESTING EQUIPMENT, INC.


11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com

## CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

- AS FOUND CHART
- AS LEFT CHART

LAB TEMPERATURE	LAB HUMIDITY	PART NUMBER	SERIAL NUMBER	SET POINT	RESULT	ALLOWABLE RANGE	CALIBRATION DATE	DUE DATE	TECHNICIAN
69.20 °F	53.10 %	165-14-3	5404340000009	930.0 °F	914.9 °F	860-1000 °F	2/11/2026	2/11/2027	SM

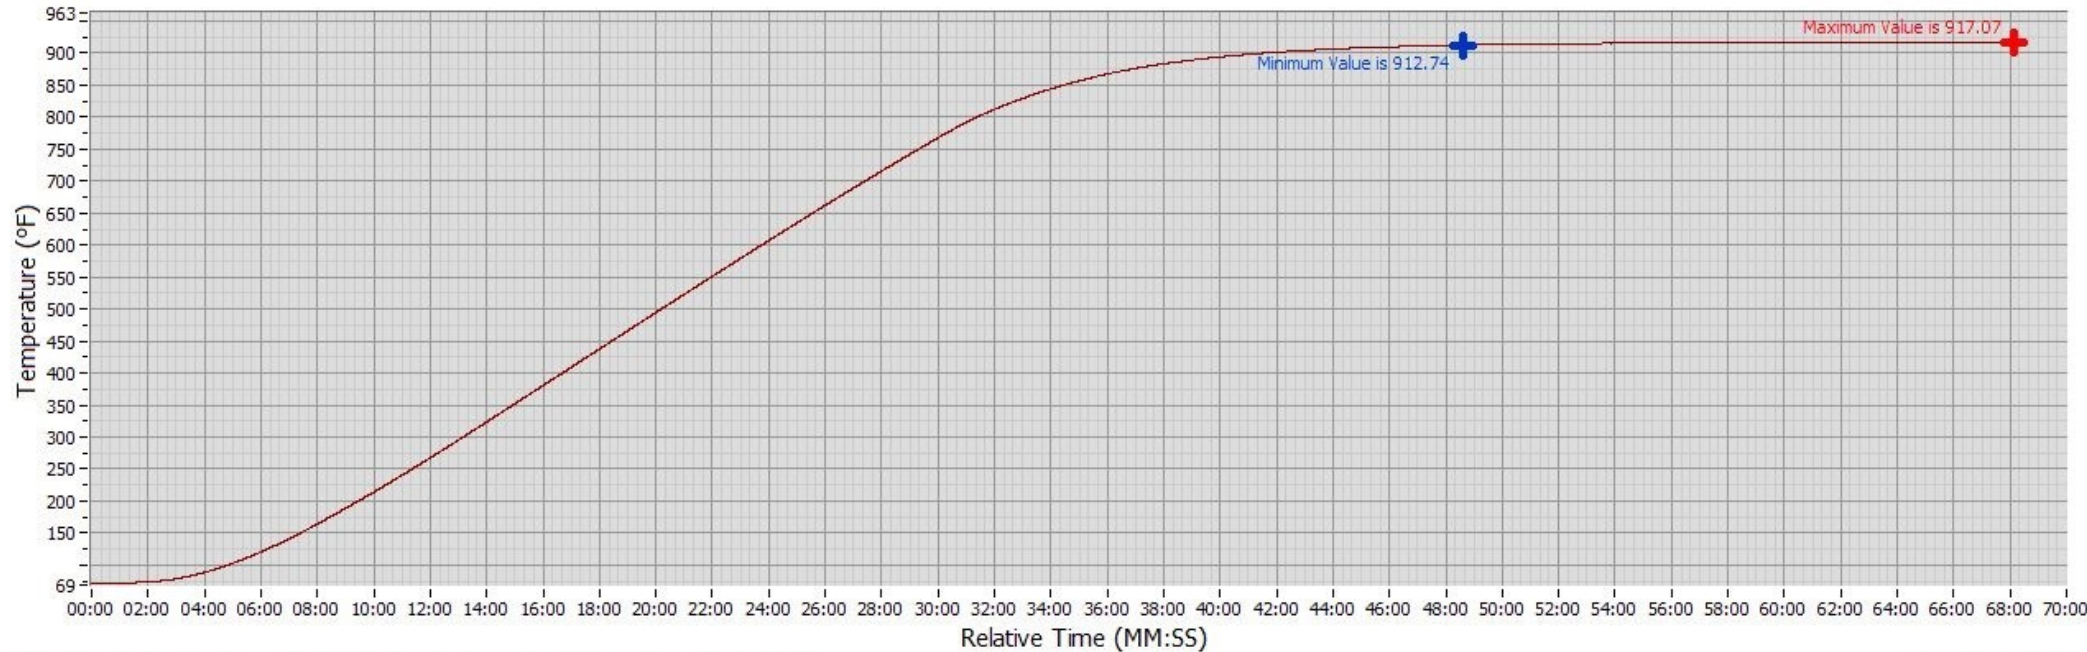

Calibration station has been calibrated using instruments which are traceable to NIST.

CAL STATION SERIAL NUMBER: 6B-11

CAL STATION CALIBRATION DATE: 11/04/2025

CAL STATION DUE DATE: 11/04/2026

AMBIENT MONITOR MODEL: RH300

AMBIENT MONITOR S/N: Z430119

AMBIENT MONITOR CAL DATE: 04/01/2025

AMBIENT MONITOR DUE DATE: 04/01/2026

UNCERTAINTY: ± 2.8°C / 5°F

CALIBRATION PROCEDURE USED: Retort Calibration Procedures API RP 13B-1

- Channel 9
- Plot 1
- Plot 2
- Plot 3
- Plot 4

AS FOUND CONDITION:

CALIBRATION RESULT: Accepted