



Dependable Products From People You Trust

OFI TESTING EQUIPMENT, INC.

11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com


CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

AS FOUND CHART

AS LEFT CHART

LAB TEMPERATURE 73.50 °F	LAB HUMIDITY 50.90 %	PART NUMBER 165-14-1	SERIAL NUMBER 540280000009	SET POINT 930.0 °F	RESULT 965.1 °F	ALLOWABLE RANGE 860-1000 °F	CALIBRATION DATE 2/13/2026	DUE DATE 2/13/2027	TECHNICIAN SM
------------------------------------	--------------------------------	--------------------------------	--------------------------------------	------------------------------	---------------------------	---------------------------------------	--------------------------------------	------------------------------	-------------------------

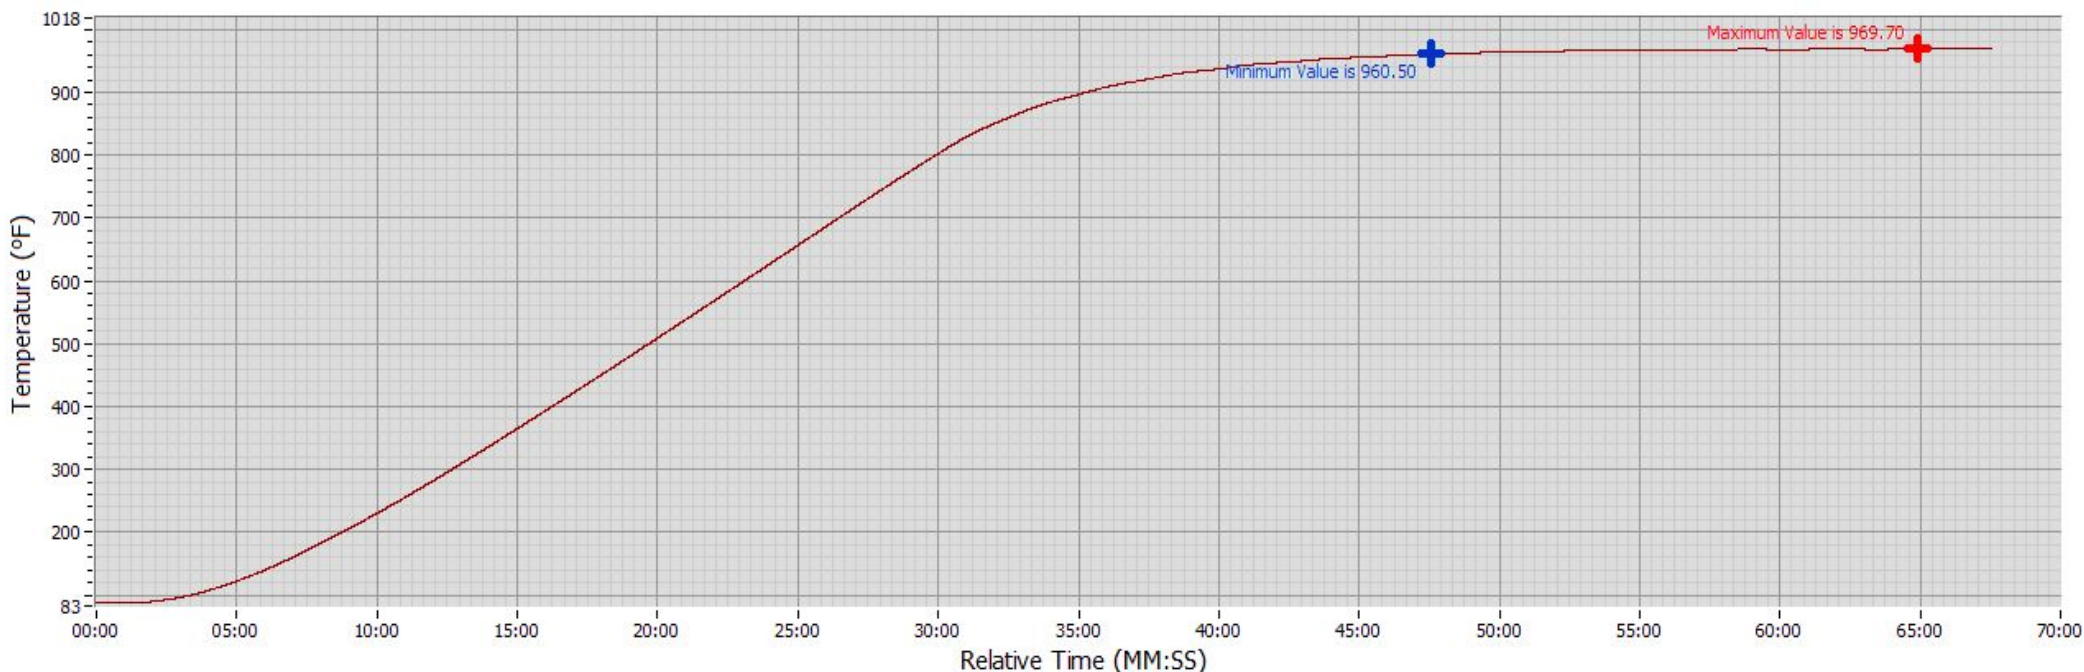

Calibration station has been calibrated using instruments which are traceable to NIST.

CAL STATION SERIAL NUMBER: 6B-11

CAL STATION CALIBRATION DATE: 11/04/2025

CAL STATION DUE DATE: 11/04/2026

AMBIENT MONITOR MODEL: RH300

AMBIENT MONITOR S/N: Z430119

AMBIENT MONITOR CAL DATE: 04/01/2025

AMBIENT MONITOR DUE DATE: 04/01/2026

UNCERTAINTY: ± 2.8°C / 5°F

CALIBRATION PROCEDURE USED: Retort Calibration Procedures API RP 13B-1

AS FOUND CONDITION:

CALIBRATION RESULT: Accepted

- Channel 1
- Plot 1
- Plot 2
- Plot 3
- Plot 4