



Roller Oven Calibration Report


Order Number:	174238
Serial # / Local I.D. #:	11-13
Calibration Date:	3/30/2026
Recommended Due Date:	3/30/2027
Certificate Number:	11-1346111
Manufacturer:	OFI Testing Equipment
Part Number:	173-00-C

Condition Found:	In Calibration
Condition Left:	In Calibration
Repairs Required:	Yes
Static Oven:	No
(F) or (C):	(°F)
Max Temp:	500
As Found Required:	No

OFI Testing Equipment, Inc. - 11302 Steeplecrest Dr - Houston, Texas - 77065 - Phone: 832.320.7300 - Web: www.ofite.com

Calibration Equipment						
Thermometer	154	EA10	Z375331	C-52617	7/23/2025	7/23/2026
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Tachometer	708	R7050	230832873	C-59865	2/3/2026	2/3/2027
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Ambient Monitor	728	RH300	Z430119	305923	4/1/2025	4/1/2026
	I.D. Number	Model Number	Serial Number	Certificate Number	Calibration Date	Calibration Due Date
Ambient Conditions	Lab / Room Temperature		73	(°F)	Lab / Room Humidity	
					38.0 %	

AS LEFT MEASUREMENTS		(°F)	Max Oven Temp	500	
Set point	Process Temperature	Accepted Deviation	Actual Deviation	Pass/Fail	
100.0	100.0	5.0	0.0	Pass	
	Pass				
200.0	202.0	5.0	2.0	Pass	
	Pass				
300.0	302.0	5.0	2.0	Pass	
	Pass				
400.0	398.0	5.0	-2.0	Pass	
	Pass				
500.0	496.0	5.0	-4.0	Pass	
	Pass				
25 RPM	25.1	2	0.1	Pass	
	Pass				
				Pass	

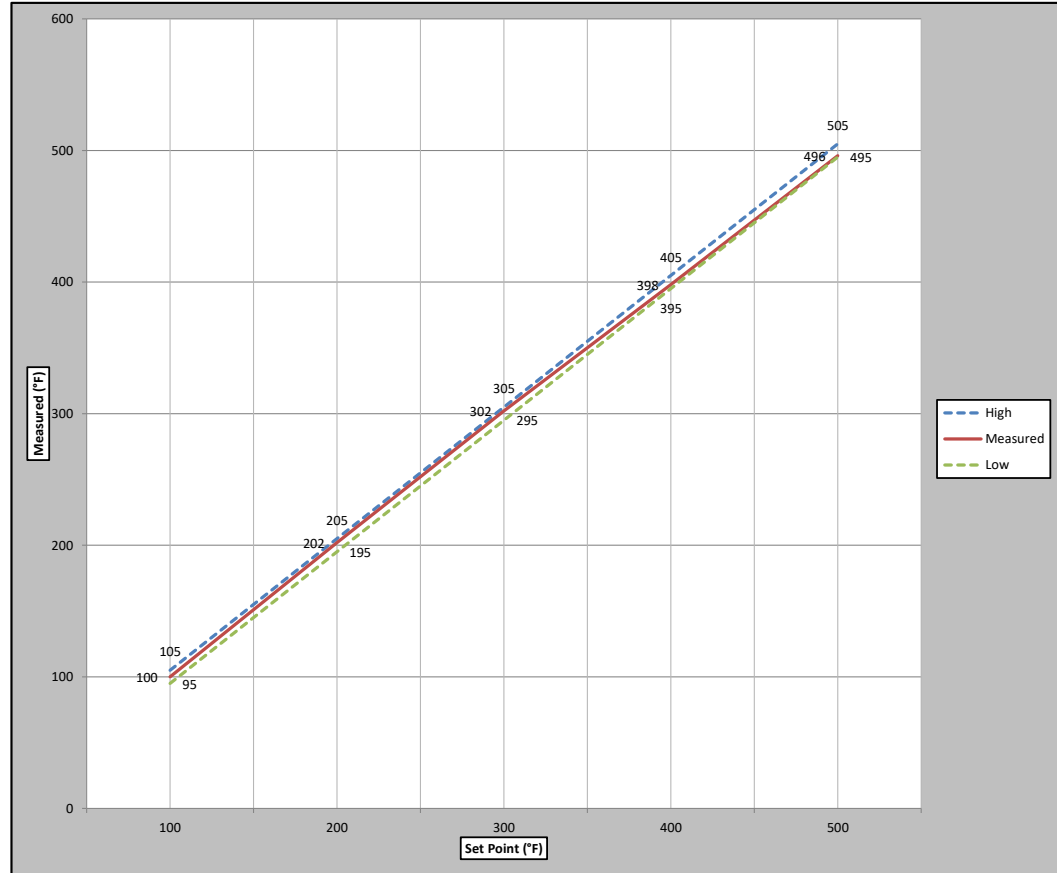

Calibration Technician: Shawn Maglito

Technician Signature: *Shawn Maglito*

Date: 3/30/2026

Reviewed By: _____

Reviewer Signature: Samantha Korenek

Review Date: 3/31/2026

Damage Report

List all damages. Describe how this could have affected measurements.

List all repairs made prior to AS LEFT measurements.

Replaced the teflon bearings holding the rollers.