



Dependable Products From People You Trust

OFI TESTING EQUIPMENT, INC.


11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com

CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

- AS FOUND CHART
- AS LEFT CHART

LAB TEMPERATURE	LAB HUMIDITY	PART NUMBER	SERIAL NUMBER	SET POINT	RESULT	ALLOWABLE RANGE	CALIBRATION DATE	DUE DATE	TECHNICIAN
75.20 °F	62.90 %	165-14-2	14-1425-003	930.0 °F	914.1 °F	860-1000 °F	4/3/2026	4/3/2027	B.T.M.

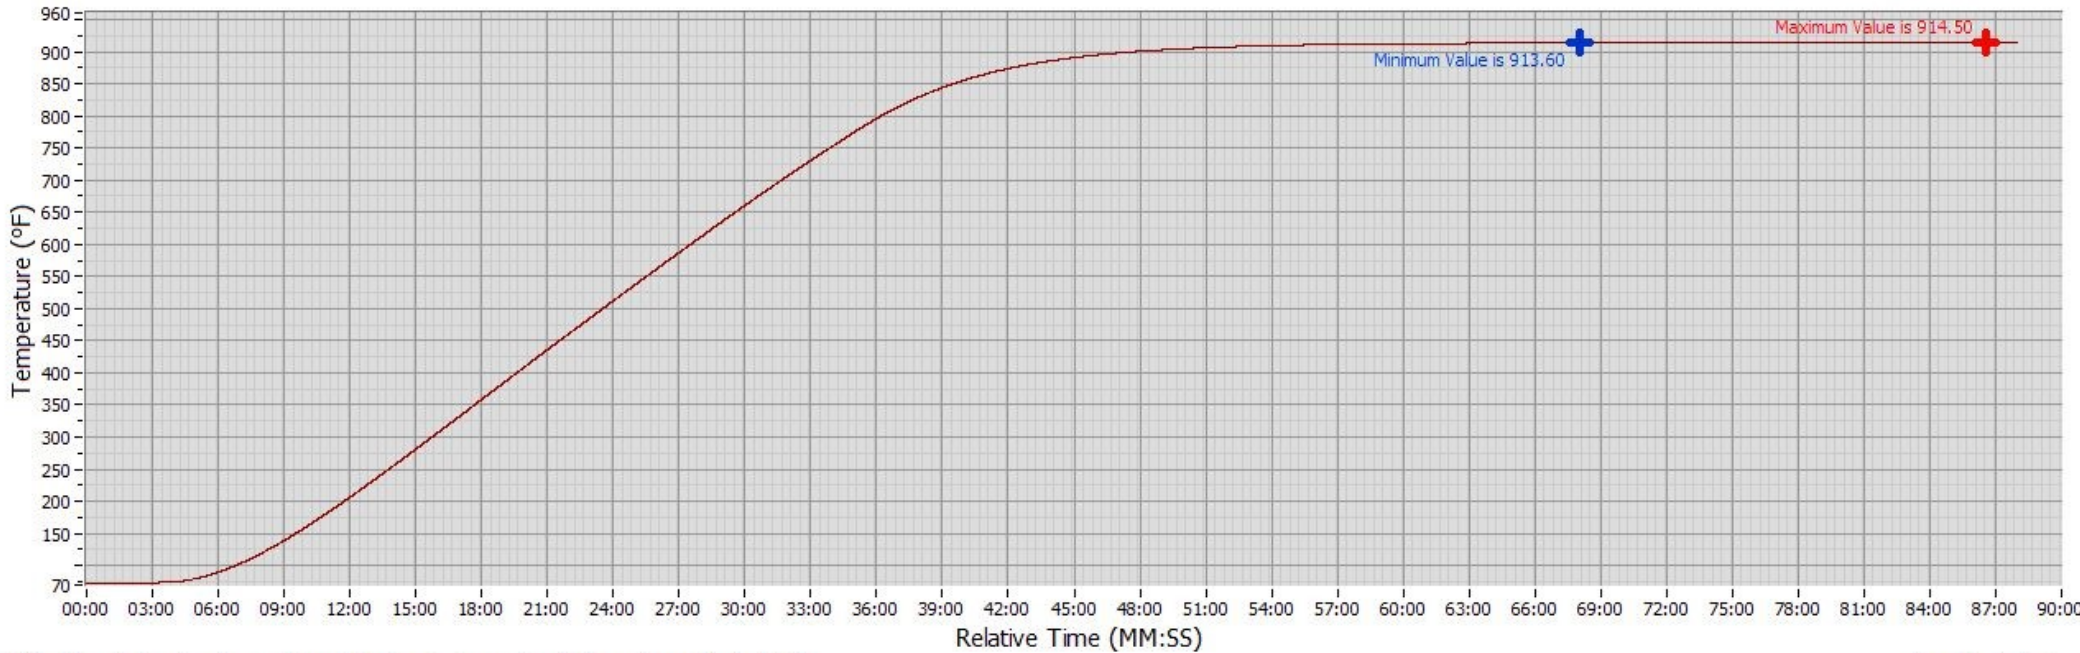

Calibration station has been calibrated using instruments which are traceable to NIST.

CAL STATION SERIAL NUMBER: 6B-11 **CAL STATION CALIBRATION DATE:** 11/04/2025 **CAL STATION DUE DATE:** 11/04/2026

AMBIENT MONITOR MODEL: RH300 **AMBIENT MONITOR S/N:** 169 **AMBIENT MONITOR CAL DATE:** 05/09/2025 **AMBIENT MONITOR DUE DATE:** 05/09/2026

UNCERTAINTY: ± 2.8°C / 5°F **CALIBRATION PROCEDURE USED:** Retort Calibration Procedures API RP 13B-1

- Channel 8
- Plot 1
- Plot 2
- Plot 3
- Plot 4

AS FOUND CONDITION:

CALIBRATION RESULT: Accepted