



Dependable Products From People You Trust

OFI TESTING EQUIPMENT, INC.

11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com


CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

AS FOUND CHART

AS LEFT CHART

LAB TEMPERATURE	LAB HUMIDITY	PART NUMBER	SERIAL NUMBER	SET POINT	RESULT	ALLOWABLE RANGE	CALIBRATION DATE	DUE DATE	TECHNICIAN
75.20 °F	62.90 %	170-00-1	5198140000007	375.0 °F	365.4 °F	350-400 °F	4/3/2026	4/3/2027	B.T.M.

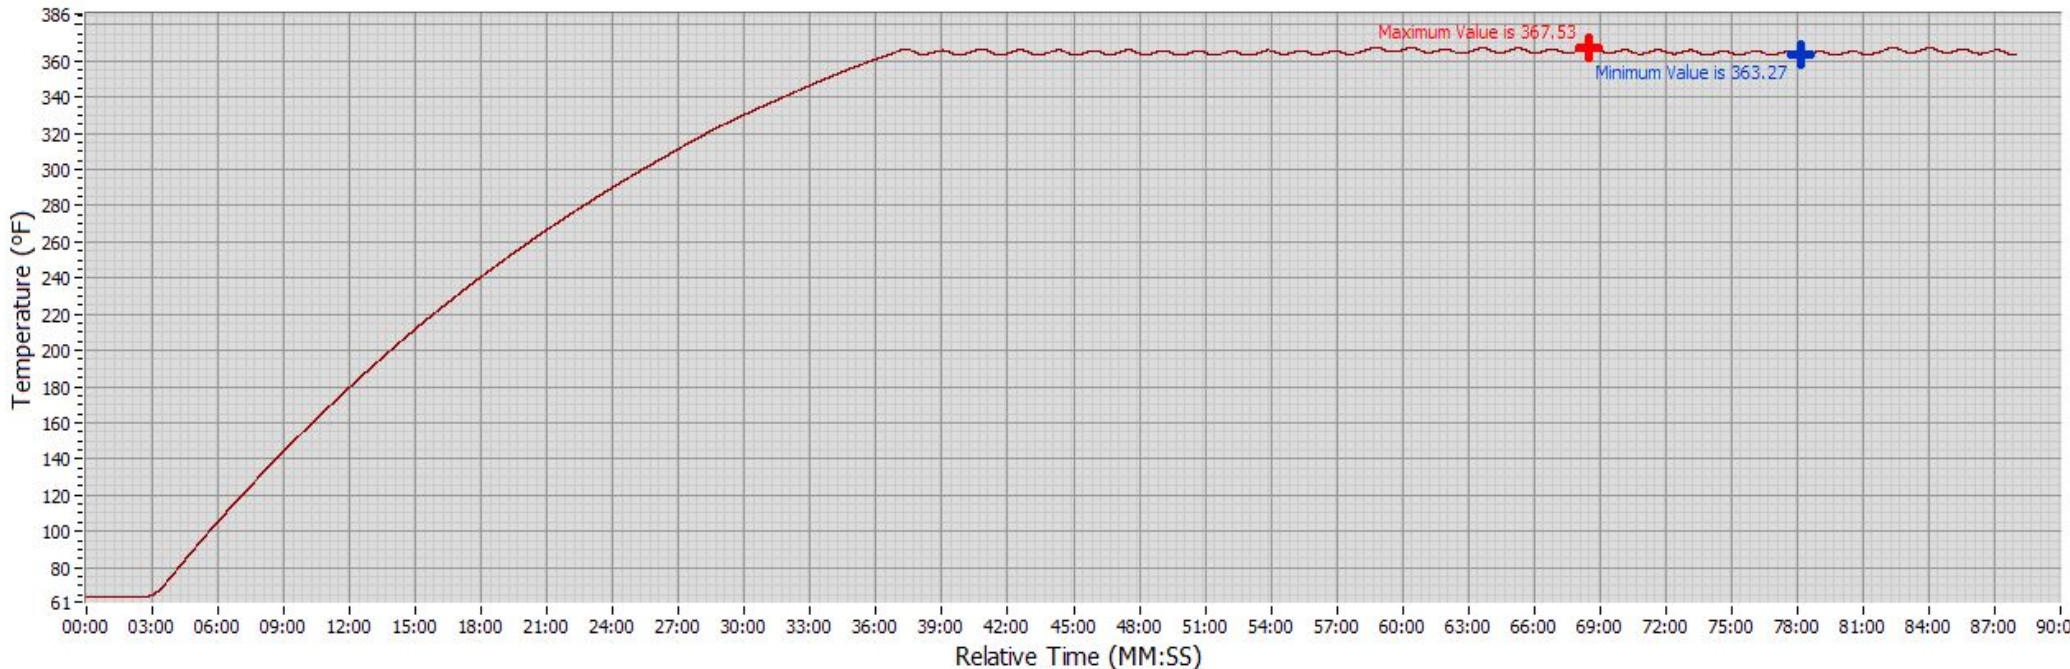

Calibration station has been calibrated using instruments which are traceable to NIST.

CAL STATION SERIAL NUMBER: 6B-11	CAL STATION CALIBRATION DATE: 11/04/2025	CAL STATION DUE DATE: 11/04/2026
AMBIENT MONITOR MODEL: RH300	AMBIENT MONITOR S/N: 169	AMBIENT MONITOR CAL DATE: 05/09/2025 AMBIENT MONITOR DUE DATE: 05/09/2026
UNCERTAINTY: ± 2.8°C / 5°F	CALIBRATION PROCEDURE USED: 175 ml Heat Jacket Calibration Procedures API RP 13B-1	

- Channel 7
- Plot 1
- Plot 2
- Plot 3
- Plot 4

AS FOUND CONDITION:

CALIBRATION RESULT: Accepted