



Dependable Products From People You Trust

OFI TESTING EQUIPMENT, INC.

11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com


CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

☐ AS FOUND CHART

☒ AS LEFT CHART

LAB TEMPERATURE	LAB HUMIDITY	PART NUMBER	SERIAL NUMBER	SET POINT	RESULT	ALLOWABLE RANGE	CALIBRATION DATE	DUE DATE	TECHNICIAN
74.10 °F	52.40 %	171-55	E005695	450.0 °F	412.6 °F	425-475 °F	7/29/2026	7/29/2027	B.T.M.

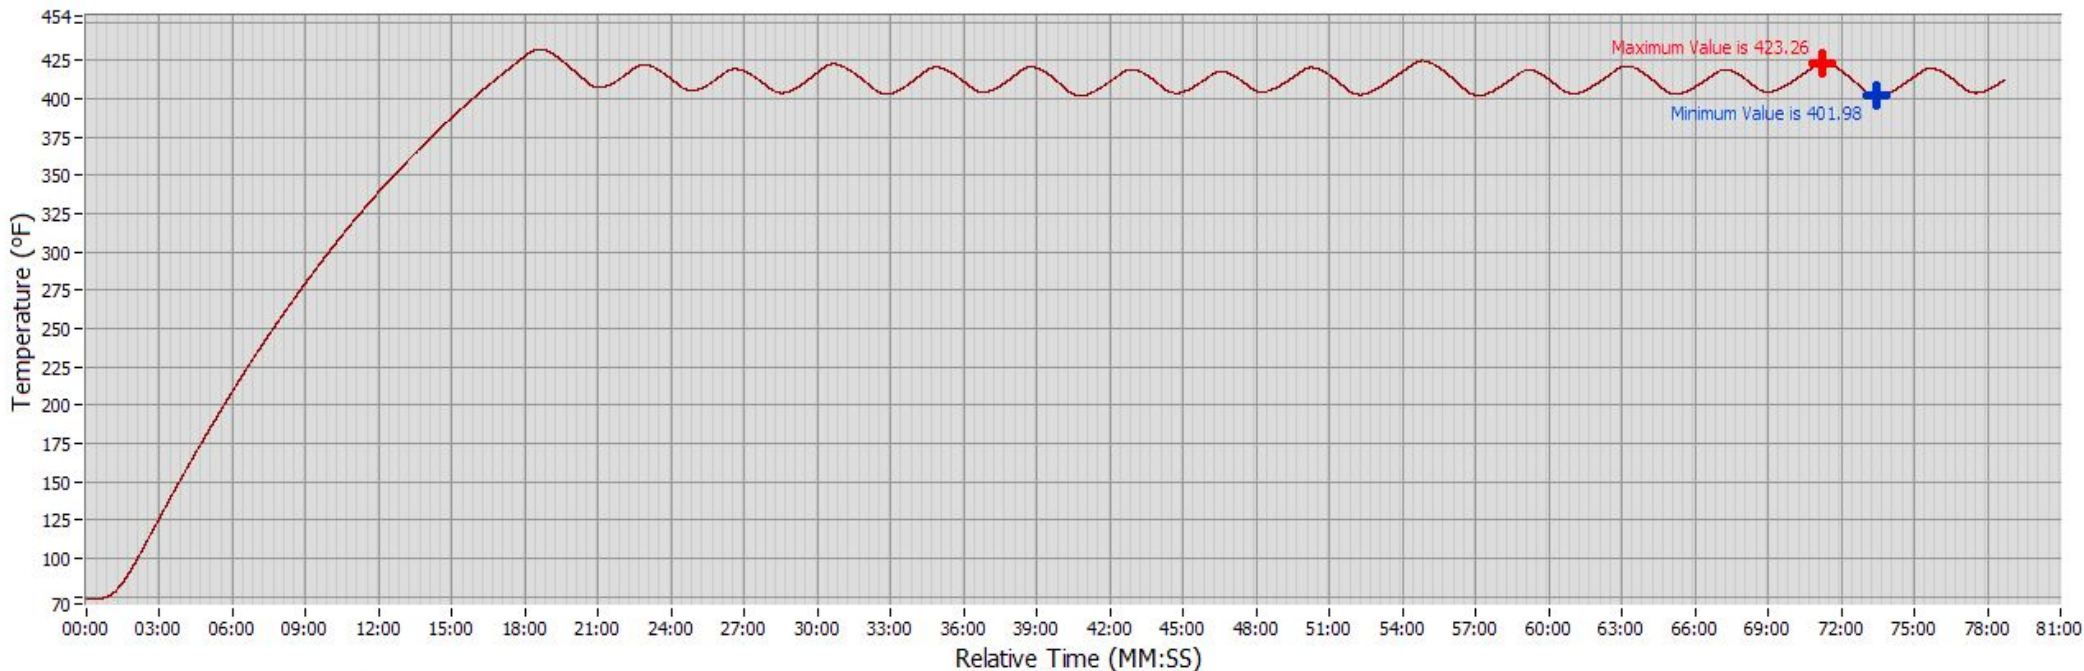

Calibration station has been calibrated using instruments which are traceable to NIST.

CAL STATION SERIAL NUMBER: 6B-11	CAL STATION CALIBRATION DATE: 11/04/2025	CAL STATION DUE DATE: 11/04/2026
AMBIENT MONITOR MODEL: RH300	AMBIENT MONITOR S/N: 728	AMBIENT MONITOR CAL DATE: 04/30/2026
AMBIENT MONITOR DUE DATE: 04/30/2027	CALIBRATION PROCEDURE USED: 500 ml Heat Jacket Calibration Procedures API RP 13B-2	
UNCERTAINTY: $\pm 2.8^{\circ}\text{C} / 5^{\circ}\text{F}$		

AS FOUND CONDITION:

CALIBRATION RESULT: Failed

Channel 1	
Plot 1	
Plot 2	
Plot 3	
Plot 4	