



Dependable Products From People You Trust


## OFI TESTING EQUIPMENT, INC.

11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com

### CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

| LAB TEMPERATURE | LAB HUMIDITY | PART NUMBER | SERIAL NUMBER | SET POINT | RESULT   | ALLOWABLE RANGE | CALIBRATION DATE | DUE DATE  | TECHNICIAN |
|-----------------|--------------|-------------|---------------|-----------|----------|-----------------|------------------|-----------|------------|
| 75.00 °F        | 53.00 %      | 170-01-1    | 52618150006   | 375.0 °F  | 371.5 °F | 350-400 °F      | 8/25/2026        | 8/25/2027 | SM         |

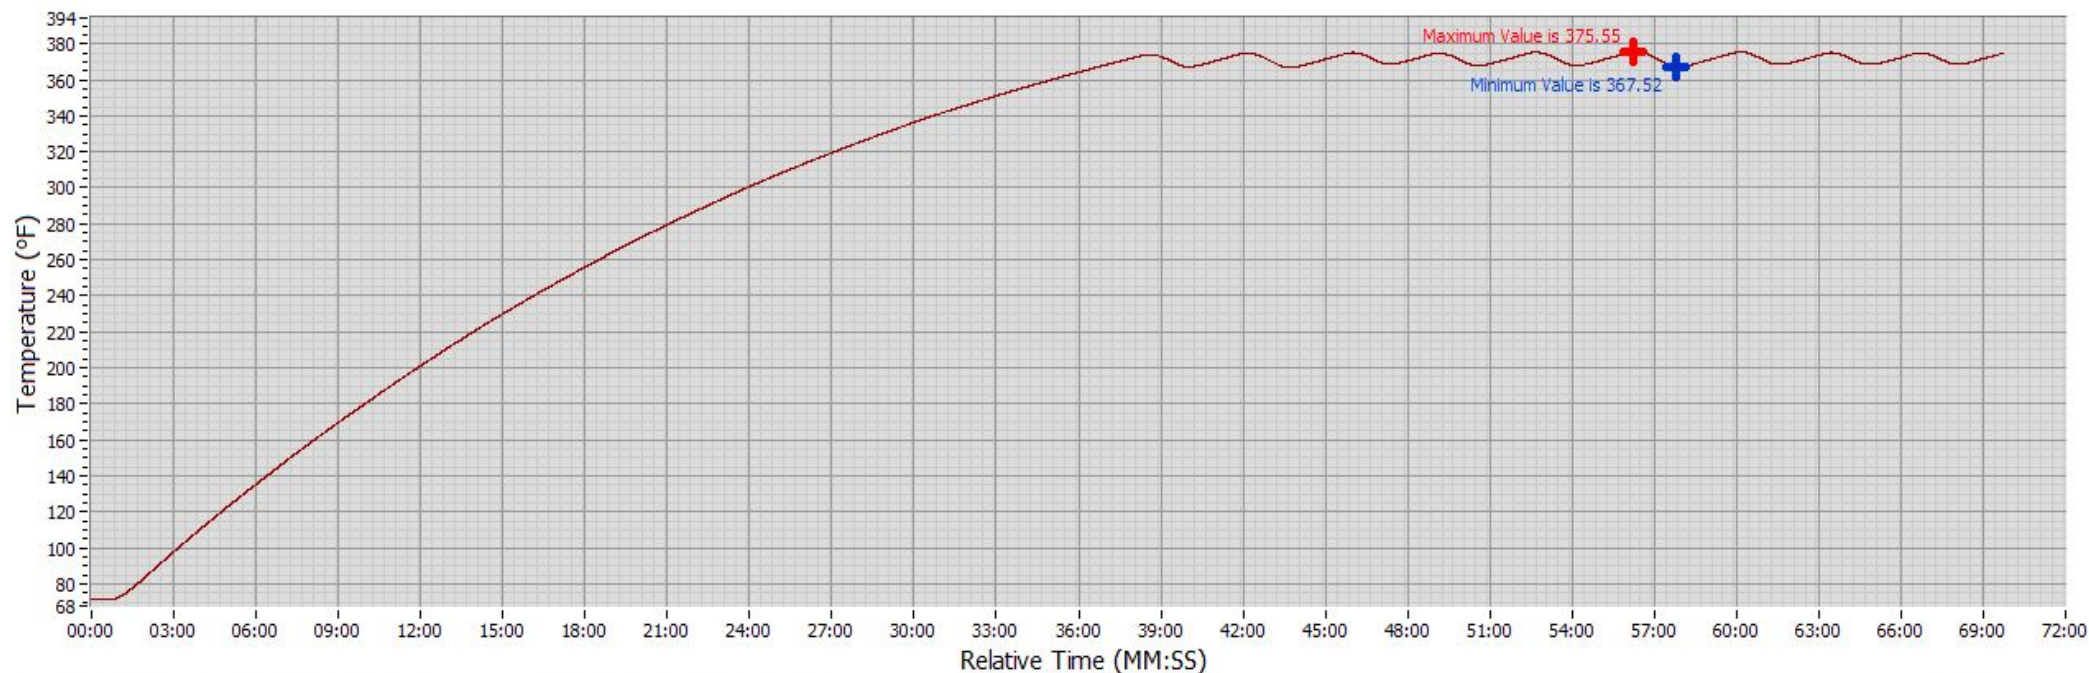

Calibration station has been calibrated using instruments which are traceable to NIST.

CAL STATION SERIAL NUMBER: 6B-11

CAL STATION CALIBRATION DATE: 11/04/2025

CAL STATION DUE DATE: 11/04/2026

AMBIENT MONITOR MODEL: RH300

AMBIENT MONITOR S/N: 728

AMBIENT MONITOR CAL DATE: 04/30/2026

AMBIENT MONITOR DUE DATE: 04/30/2027

UNCERTAINTY:  $\pm 2.8^{\circ}\text{C} / 5^{\circ}\text{F}$

CALIBRATION PROCEDURE USED: 175 ml Heat Jacket Calibration Procedures API RP 13B-1

AS FOUND CONDITION:

CALIBRATION RESULT: Accepted

|           |  |
|-----------|--|
| Channel 6 |  |
| Plot 1    |  |
| Plot 2    |  |
| Plot 3    |  |
| Plot 4    |  |