



OFI Testing Equipment, Inc.
11302 Steeplecrest Drive Houston, TX 77065 USA
Phone: 832-320-7300 · Fax: 713-880-9886 · Web: www.ofite.com

Roller Oven Series Calibration Report

Repairs Required? No

As Found Data Required by Customer? No

Static Oven: No

(°F) or (°C) : (°F)

Part Number: 173-00-C

Manufacturer: OFI Testing Equipment

Serial Number: 01128

S/O# or I/O# SV00000068

Master Testing Equipment

Thermometer: 257 Model #: EA10 Serial #: Z375329 Calibration Due: 2/25/2027 Tachometer: 679 Model #: R7050 Serial #: 220326766 Calibration Due: 7/17/2027

Ambient Conditions

Ambient Monitor: 261 Model No: EA20

Calibration Date: 1/20/2026

Calibration Due: 1/20/2027

Serial No: Z375174

Ambient Conditions: Room Temperature: 70

Relative Humidity: 49

AS LEFT MEASUREMENTS		(°F)		
Set point	Process Temperature	Accepted Deviation	Actual Deviation	Pass/Fail
100	100	5	0	Pass
200	202	5	2	Pass
300	299	5	-1	Pass
400	395	5	-5	Pass
25 RPM	25.3	2	0.3	Pass
				Pass

Technician: Arnulfo Muniz


Calibration Date: 9/1/2026

Recommended Calibration Date *: 9/1/2027

* To be provided by customer

Reviewed By: Antonio Rico

Review Date: 9/2/2026

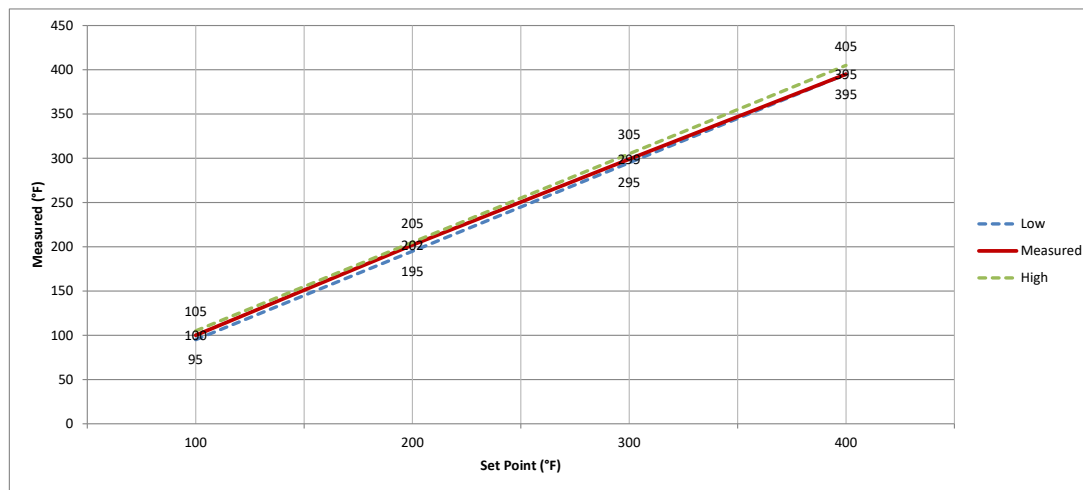

Revised 01/25/2023

This report meets or exceeds the requirements outlined in API RP 13B-1 Recommended Practice for Field Testing Water-based Drilling Fluids and API RP 13B-2 Recommended Practice for Field Testing Oil-based Drilling Fluids for calibration of laboratory devices, using certified master test equipment that is traceable to NIST.