



Dependable Products From People You Trust

OFI TESTING EQUIPMENT, INC.

11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com


CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

☐ AS FOUND CHART

☒ AS LEFT CHART

LAB TEMPERATURE	LAB HUMIDITY	PART NUMBER	SERIAL NUMBER	SET POINT	RESULT	ALLOWABLE RANGE	CALIBRATION DATE	DUE DATE	TECHNICIAN
72.00 °F	47.00 %	171-00	14-401	500.0 °F	496.9 °F	485-550 °F	9/1/2026	9/1/2027	Amir Mek

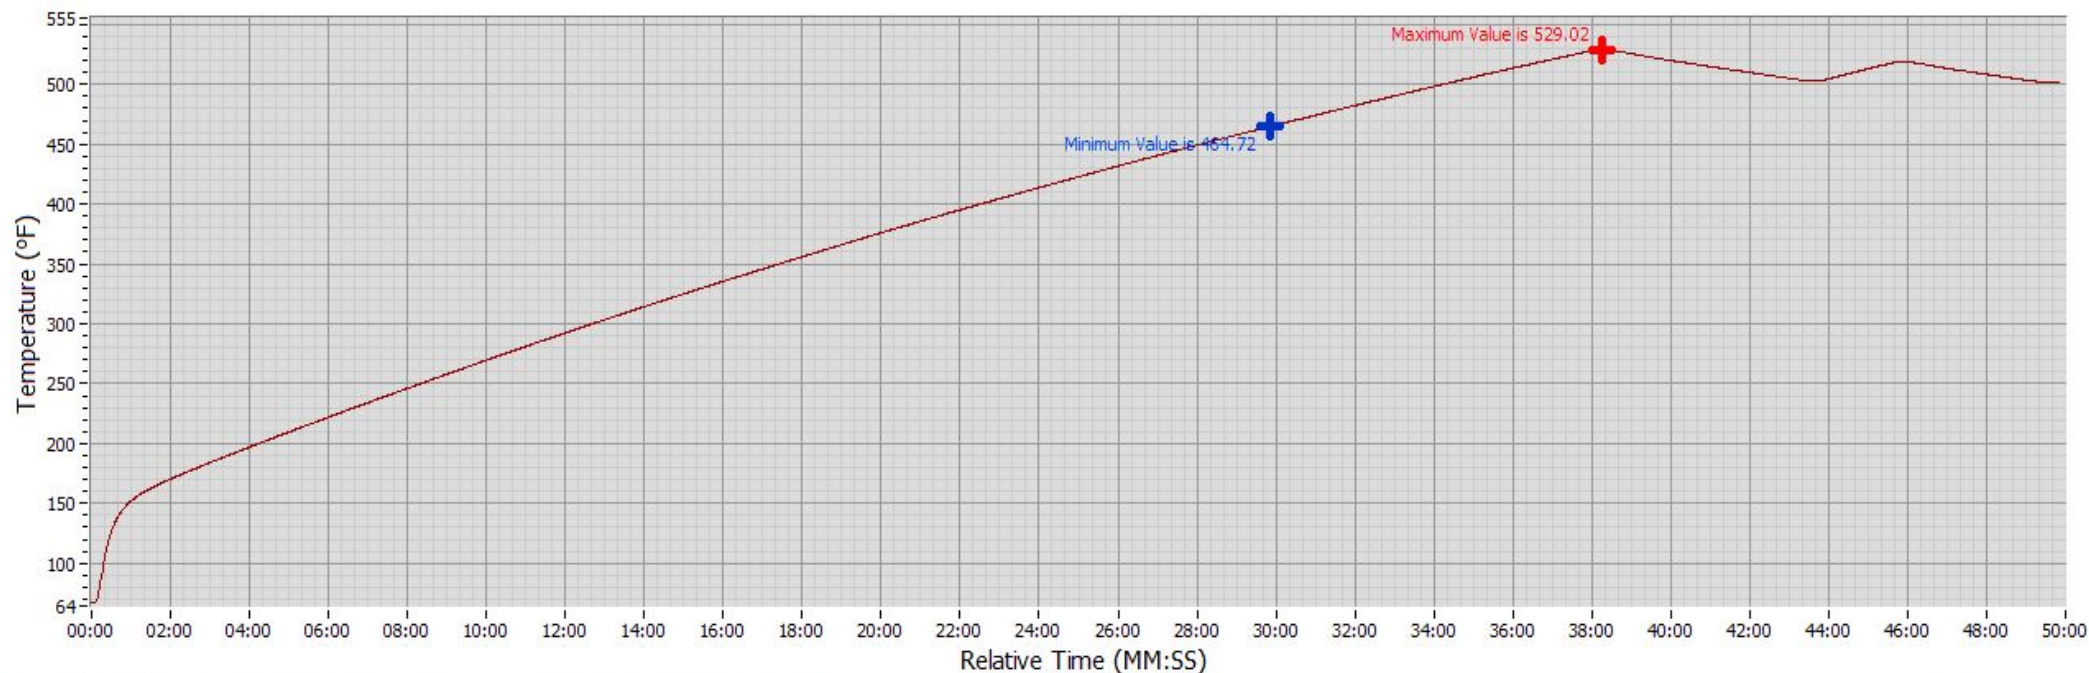

Calibration station has been calibrated using instruments which are traceable to NIST.

CAL STATION SERIAL NUMBER: 6B-11

CAL STATION CALIBRATION DATE: 06/19/2026

CAL STATION DUE DATE: 06/19/2027

AMBIENT MONITOR MODEL: EV20

AMBIENT MONITOR S/N: Z375329

AMBIENT MONITOR CAL DATE: 05/20/2026

AMBIENT MONITOR DUE DATE: 05/20/2027

UNCERTAINTY: $\pm 2.8^{\circ}\text{C} / 5^{\circ}\text{F}$

CALIBRATION PROCEDURE USED:

AS FOUND CONDITION:

CALIBRATION RESULT: Accepted

Channel 1

Plot 1

Plot 2

Plot 3

Plot 4