



Dependable Products From People You Trust


## OFI TESTING EQUIPMENT, INC.

11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com

### CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

| LAB TEMPERATURE | LAB HUMIDITY | PART NUMBER | SERIAL NUMBER | SET POINT | RESULT   | ALLOWABLE RANGE | CALIBRATION DATE | DUE DATE | TECHNICIAN |
|-----------------|--------------|-------------|---------------|-----------|----------|-----------------|------------------|----------|------------|
| 74.00 °F        | 49.00 %      | 165-14-3    | 52617980009   | 930.0 °F  | 918.3 °F | 860-1000 °F     | 9/8/2026         | 9/8/2027 | SM         |

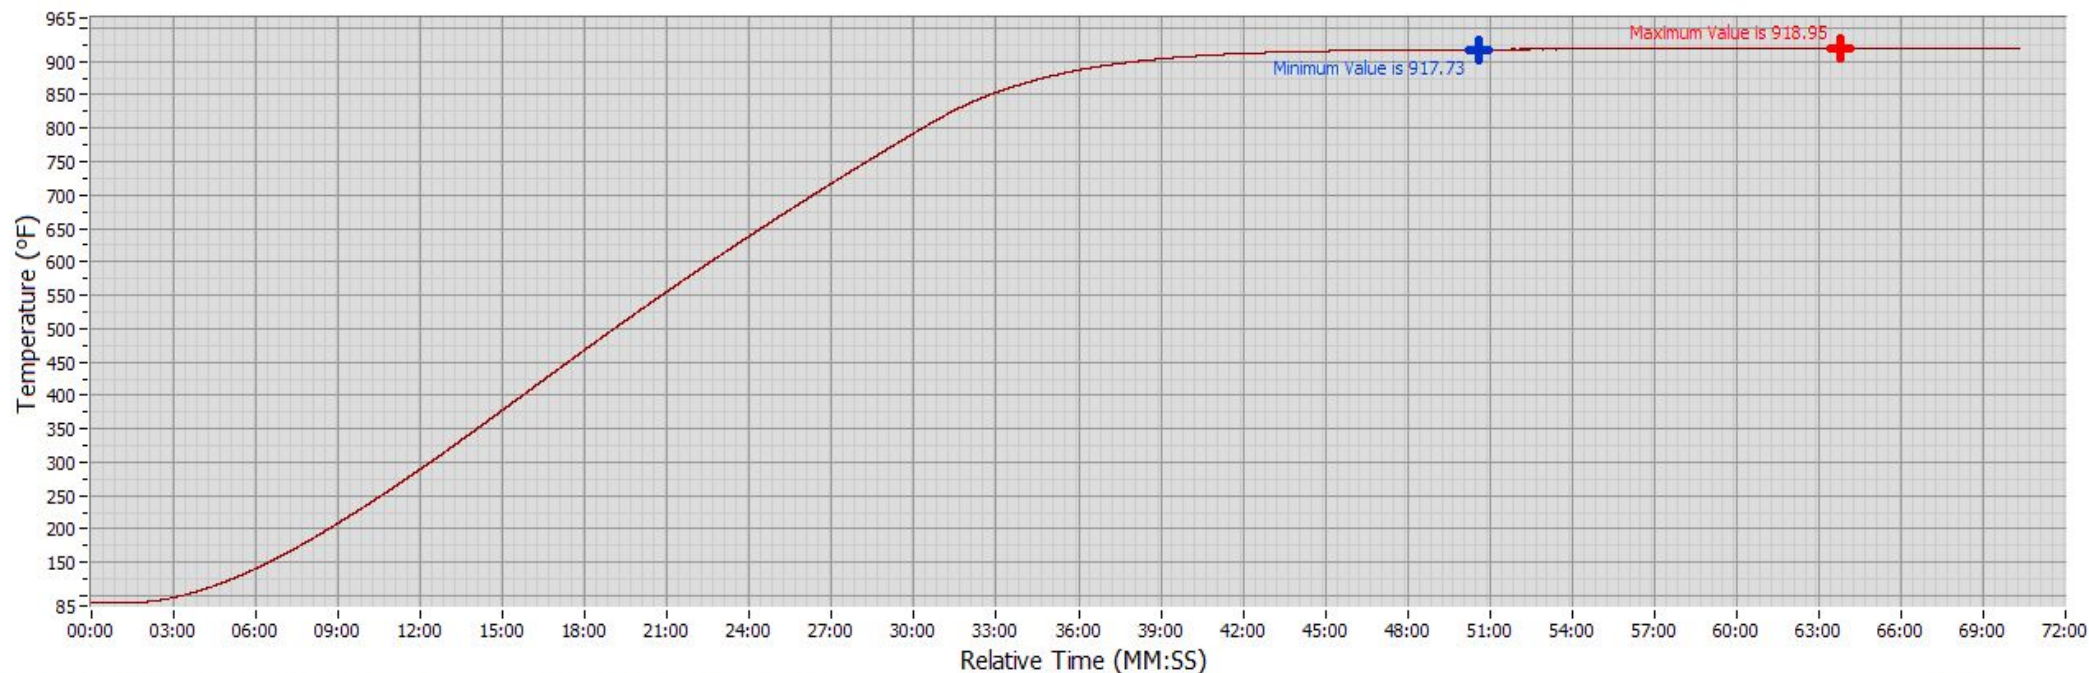

Calibration station has been calibrated using instruments which are traceable to NIST.

CAL STATION SERIAL NUMBER: 6B-11

CAL STATION CALIBRATION DATE: 11/04/2025

CAL STATION DUE DATE: 11/04/2026

AMBIENT MONITOR MODEL: RH300

AMBIENT MONITOR S/N: 728

AMBIENT MONITOR CAL DATE: 04/30/2026

AMBIENT MONITOR DUE DATE: 04/30/2027

UNCERTAINTY:  $\pm 2.8^{\circ}\text{C} / 5^{\circ}\text{F}$

CALIBRATION PROCEDURE USED: Retort Calibration Procedures API RP 13B-1

AS FOUND CONDITION:

CALIBRATION RESULT: Accepted

|           |  |
|-----------|--|
| Channel 4 |  |
| Plot 1    |  |
| Plot 2    |  |
| Plot 3    |  |
| Plot 4    |  |