

- ☐ AS FOUND CHART
- ☒ AS LEFT CHART



Dependable Products From People You Trust


# OFI TESTING EQUIPMENT, INC.

11302 Steeplecrest Drive, Houston, Texas 77065 Phone (832) 320-7300 Fax (713) 880-9886 Web www.ofite.com

## CALIBRATION CERTIFICATE

Temperatures are calibrated to meet or exceed the requirements stated in API RP 13B-1 and API RP 13B-2

| LAB TEMPERATURE | LAB HUMIDITY | PART NUMBER | SERIAL NUMBER | SET POINT | RESULT   | ALLOWABLE RANGE | CALIBRATION DATE | DUE DATE | TECHNICIAN |
|-----------------|--------------|-------------|---------------|-----------|----------|-----------------|------------------|----------|------------|
| 75.00 °F        | 52.00 %      | 165-14-3    | 52617990009   | 930.0 °F  | 921.8 °F | 860-1000 °F     | 9/9/2026         | 9/9/2027 | SM         |

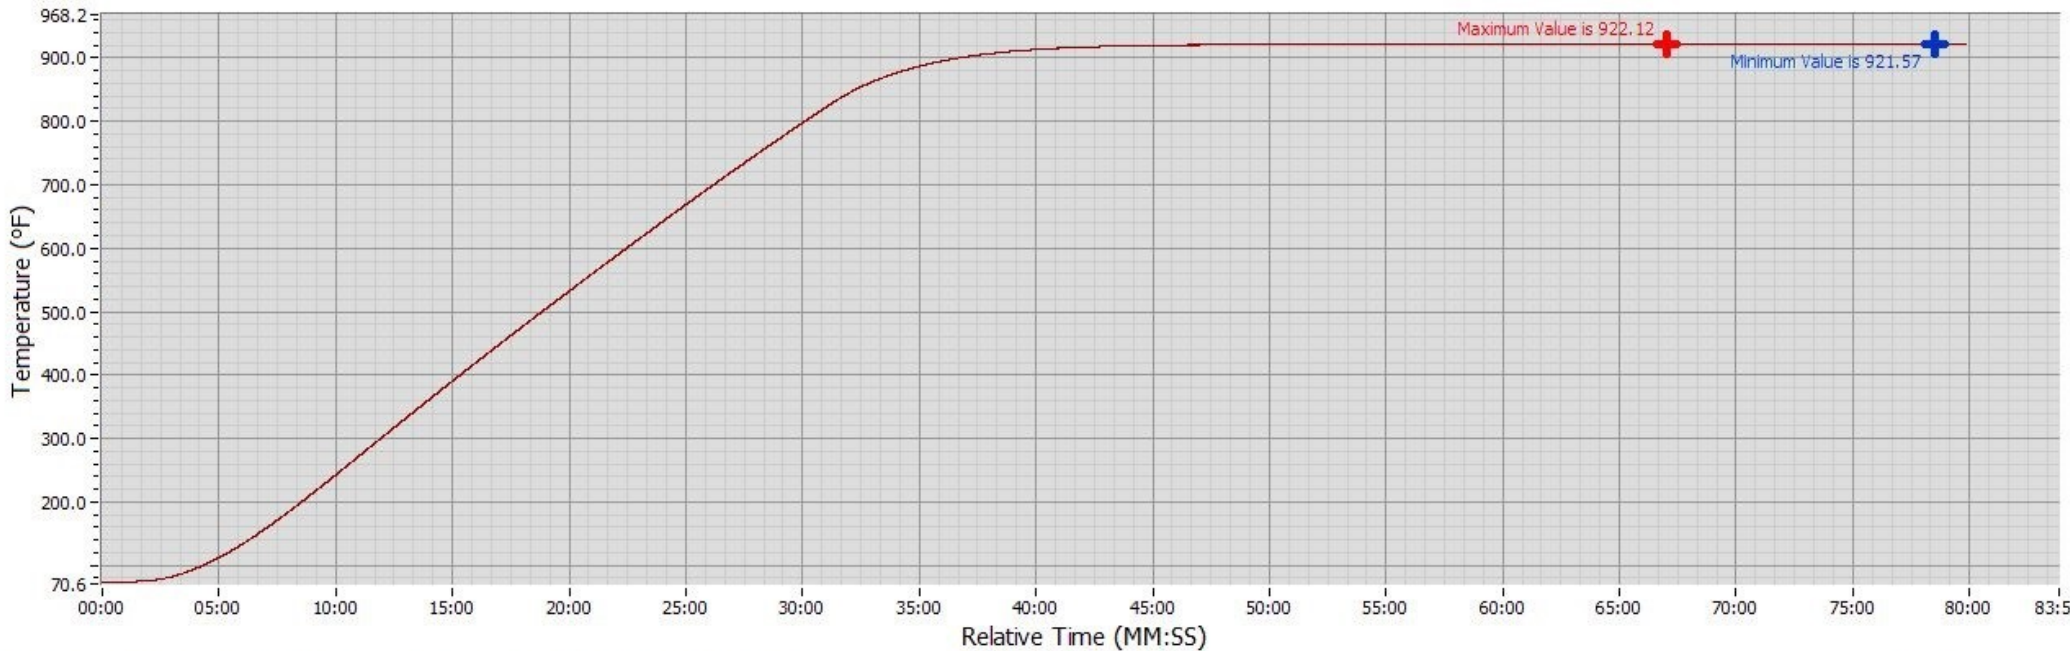

Calibration station has been calibrated using instruments which are traceable to NIST.

**CAL STATION SERIAL NUMBER:** 6B-11

**CAL STATION CALIBRATION DATE:** 11/04/2025

**CAL STATION DUE DATE:** 11/04/2026

**AMBIENT MONITOR MODEL:** RH300

**AMBIENT MONITOR S/N:** 728

**AMBIENT MONITOR CAL DATE:** 04/30/2026

**AMBIENT MONITOR DUE DATE:** 04/30/2027

**UNCERTAINTY:** ± 2.8°C / 5°F

**CALIBRATION PROCEDURE USED** Retort Calibration Procedures API RP 13B-1

AS FOUND CONDITION:

CALIBRATION RESULT: Accepted